


TECHNICAL MANUAL

OPERATOR'S, UNIT,
DIRECT SUPPORT AND
GENERAL SUPPORT
MAINTENANCE MANUAL
FOR

**SHELTER, ELECTRICAL
EQUIPMENT S-280B/G
(NSN 5411-00-117-2868)**

**S-280B/G (SHIELDED)
(NSN 5411-00-001-4093)**

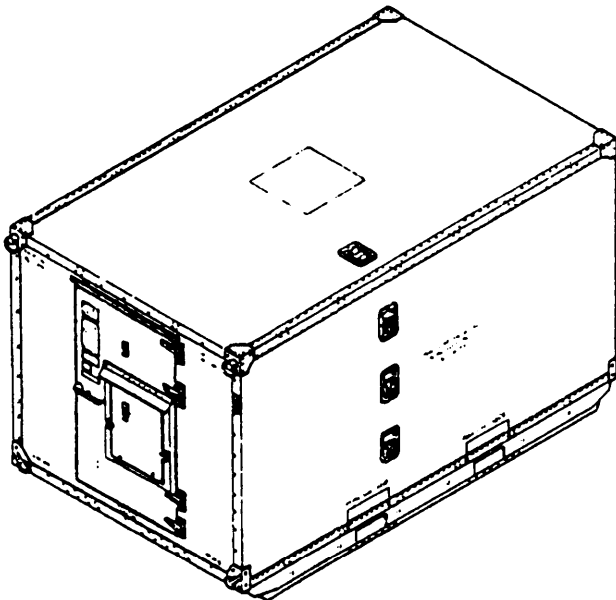

INTRODUCTION 1-1

OPERATOR PMCS 2-1

UNIT MAINTENANCE
INSTRUCTIONS 3-1

DIRECT SUPPORT
MAINTENANCE INSTRUCTIONS 4-1

GENERAL SUPPORT
MAINTENANCE INSTRUCTIONS 5-1

REFERENCES A-1

MAINTENANCE ALLOCATION CHART B-1

COMPONENTS OF END ITEM AND BASIC
ISSUE ITEMS LISTS C-1

EXPENDABLE/DURABLE SUPPLIES AND
MATERIALS LIST D-1

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

HEADQUARTERS, DEPARTMENT OF THE ARMY
30 SEPTEMBER 1993

WARNING

Drilling creates metal chips which may enter eyes and cause serious injury. Eye protection is required.

Adhesives and solvents are flammable and toxic. Keep away from heat and open flames. Use in a well-ventilated area. Avoid skin and eye contact and breathing of vapors. Use protective goggles and gloves. Use in accordance with manufacturer's instructions.

CHANGE
NO. 1

HEADQUARTERS, DEPARTMENT OF THE ARMY
WASHINGTON, DC, 31 AUGUST 2005

TECHNICAL MANUAL

OPERATOR'S, UNIT, DIRECT SUPPORT AND GENERAL SUPPORT MAINTENANCE
MANUAL

FOR
SHELTER, ELECTRICAL EQUIPMENT

S-280B/G	NSN: 5411-00-117-2868
S-280B/G (SHEILDED)	NSN: 5411-00-001-4093

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

TM 10-5411-206-14, 30 September 1993, is updated as follows:

1. File this sheet in front of the manual for reference.
2. This change implements Army Maintenance Transformation and changes the Maintenance Allocation Chart (MAC) to support Field and Sustainment Maintenance.
3. New or updated change information is indicated by a vertical bar in the outer margin of the page.
4. Remove old pages and insert new pages as indicated below:

Remove Pages

Insert Pages

B-1 through B-6

A/(B Blank)

B-1 through B-7/(B-8 Blank)

Electronic 2028 Instructions

Sample 2028

Sample 2028 Front/Back

2028 Front/Back


2028 Front/Back

2028 Front/Back

By Order of the Secretary of the Army:

PETER J. SCHOOMAKER
General, United States Army
Chief of Staff

Official:


SANDRA R. RILEY
*Administrative Assistant to the
Secretary of the Army*
0521012

Distribution: To be distributed in accordance with initial distribution number (IDN) 256169 requirements for TM 10-5411-206-14.

INSERT LATEST CHANGED PAGES. DESTROY SUPERSEDED PAGES.

LIST OF EFFECTIVE PAGES

NOTE: The portion of text affected by the update is indicated by a vertical line in the outer margins of the page.
Updates to illustrations are indicated by shaded or screened areas, or by miniature pointing hands.

Dates of issue for original and changed pages / work packages are:

Original .. 0 .. 30 Sep 93

Change .. 1 .. 31 Aug 05

TOTAL NUMBER OF PAGES FOR THIS PUBLICATION IS 136, CONSISTING OF THE FOLLOWING:

Page No.	*Change No.
Title	0
a/(b Blank)	0
i through iv	0
1-1 through 1-4	0
2-1 through 2-6	0
3-1 through 3-35/(3-36 Blank)	0
4-1 through 4-25/(4-26 Blank)	0
5-1 through 5-15/(5-16 Blank)	0
A-1/(A-2 Blank)	0
B-1 through B-7/(B-8 Blank)	1
C-1 through C-3/(C-4 Blank)	0
D-1 through D-3/(D-4 Blank)	0
Index 1 through Index 4/(Index 5 Blank)	0

***Zero in this column indicates an original page**

TECHNICAL MANUAL

No. 10-5411-206-14

HEADQUARTERS
DEPARTMENT OF THE ARMY
WASHINGTON D. C., 30 September 1993

**Operator's, Unit, Direct Support and General Support
Maintenance Manual
for
SHELTER, ELECTRICAL EQUIPMENT
S-280B/G (NSN 5411-00-117-2868)
S-280 B/G (Shielded) (NSN 5411-00-001-4093)**

REPORTING ERRORS AND RECOMMENDING IMPROVEMENTS

You can help improve this manual. If you find any mistakes or if you know of a way to improve the procedures, please let us know. Mail your letter or DA Form 2028 (Recommended Changes to Publications and Blank Forms), or DA Form 2028-2 located in the back of this manual directly to: Commander, US Army Aviation and Troop Command, ATTN: AMSAT-I-MP, 4300 Goodfellow Blvd., St. Louis, MO 63120-1798. A reply will be furnished directly to you.

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

TABLE OF CONTENTS

		Page
CHAPTER I	<u>INTRODUCTION</u>	1-1
Section I	General Information	1-1
Section II	Equipment Description	1-2
CHAPTER 2	OPERATING INSTRUCTIONS	2-1
Section I	<u>Operator Preventive Maintenance Checks and Services (PMCS)</u>	2-1
Section II	Operation Under Usual Conditions	2-4
Section III	Operation Under Unusual Conditions	2-6
CHAPTER 3	<u>UNIT MAINTENANCE INSTRUCTIONS</u>	3-1
Section I	Lubrication	3-1
Section II	Repair Parts, Special Tools, TMDE and Support Equipment	3-1
Section III	Service Upon Receipt	3-1
Section IV	Troubleshooting	3-4
Section V	Unit Maintenance Procedures	3-7
Section VI	Preparation for Shipment and Storage	3-35

TABLE OF CONTENTS (cont)

	Page
CHAPTER 4	<u>DIRECT SUPPORT MAINTENANCE INSTRUCTIONS</u> 4-1
Section I	Repair Parts, Special Tools, TMDE and Support Equipment 4-1
Section II	Troubleshooting 4-1
Section III	Direct Support Maintenance Procedures 4-3
CHAPTER 5	<u>GENERAL SUPPORT MAINTENANCE INSTRUCTIONS</u> 5-1
Section I	Repair Parts, Special Tools, TMDE and Support Equipment 5-1
Section II	General Support Maintenance Procedures 5-1
APPENDIX A	<u>REFERENCES</u> A-1
APPENDIX B	<u>MAINTENANCE ALLOCATION</u> B-1
APPENDIX C	<u>COMPONENTS OF END ITEM AND BASIC ISSUE ITEMS</u> C-1
APPENDIX D	<u>EXPENDABLE AND DURABLE SUPPLIES AND MATERIALS LIST</u> D-1
INDEX I-1

LIST OF ILLUSTRATIONS

Figure Number	Title	Page
1-1	Major Shelter Components	1-3
1-2	Shelter Marking	1-4
2-1	Instruction and Warning Plates	2-5
3-1	Lifting and Loading Shelter	3-3
3-2	Securing Shelter on 21/2 Ton Truck	3-5
3-3	Rivet Types	3-9
3-4	Installing Blind Rivets	3-11
3-5	Removing Blind Rivets	3-13
3-6	Rivnuts (Threaded Inserts)	3-13
3-7	Installing Rivnuts	3-14
3-8	Removing Rivnuts	3-16
3-9	Door Brace Assembly Removal and Disassembly	3-19
3-10	Door Brace Assembly Reassembly and installation	3-20
3-11	Emergency Exit panel Assembly Replacement	3-22
3-12	T-Latch and Holder Replacement	3-23
3-13	Door Latch Assembly Removal and Disassembly	3-25
3-14	Door Latch Assembly Reassembly and Installation	3-27
3-15	Air inlet Filter Replacement	3-30
3-16	Recessed Step Pan Assembly Replacement	3-31
3-17	D-Ring Assembly Replacement	3-33
3-18	Drain Plug and EMI Washer Replacement	3-34
4-1	Drip Mold Replacement	4-4
4-2	Data Plate Replacement	4-5
4-3	Door Stop Angle Replacement	4-6
4-4	Weather Gasket Replacement	4-10
4-5	Drip Cap Replacement	4-11
4-6	Emergency Exit Latch, Strike and Stud Plate Assembly Replacement	4-13
4-7	intake Louver Assembly and RFI/EMI Filter Replacement	4-15
4-8	Door Knob Assembly Replacement	4-17
4-9	Door Hinge Assembly Replacement	4-19
4-10	Panel Repair	4-25
5-1	Door Assembly Replacement	5-3
5-2	Towing Eye Assembly Repair and Replacement	5-5
5-3	Lifting Eye Assembly Repair and Replacement	5-7
5-4	RFI/EMI Shielding Gasket Replacement	5-9
5-5	Panel Repair	5-13
5-6	Skid Assembly and Mounting Bracket Replacement	5-15

LIST OF TABLES

Table Number	Title	Page
2-1	Operator Preventive Maintenance Checks and Services	2-2
3-1	Troubleshooting	3-6
3-2	Blind Rivets	3-9
3-3	Rivnuts	3-14
4-1	Troubleshooting	4-2

HOW TO USE THIS MANUAL

This manual is designed to help you keep your shelter in good operating condition. The front cover index is provided for quick reference to important information. There is also an index located in the final pages for use in locating specific items of information.

Warning pages are located in the front of this manual. You should learn the warnings before Performing any maintenance on the equipment.

Paragraphs in this manual are numbered by chapter and order of appearance within a chapter. A subject index appears at the beginning of each chapter listing sections that are included in that chapter. A more specific subject index is located at the beginning of each section to help you find the exact paragraph you are looking for.

CHAPTER 1

INTRODUCTION

Subject	Section	Page
General Information	I	1-1
Equipment Description	II	1-2

Section I. GENERAL INFORMATION

Subject	Para	Page
Scope	1-1	1-1
Maintenance Forms and Records	1-2	1-1
Reporting Equipment Improvement Recommendations	1-3	1-1
Destruction of Army Materiel to Prevent Enemy Use	1-4	1-1
Preparation for Shipment and Storage	1-5	1-2
List of Abbreviations	1-6	1-2

1-1. **Scope.**

a. Type of Manual. This technical manual includes operator, unit, direct support and general support maintenance procedures for the basic S-280B/G and S-280B/G Shielded shelters. Additional maintenance data relevant to a configured shelter can be found in the applicable end item technical manual.

b. Equipment Name and Model Number. This technical manual covers electrical Equipment Shelters S-280B/G. Some configurations of the S-280B/G shelter are equipped with radio frequency/electromagnetic interference shielding.

c. Purpose of Equipment. The S-280B/G and S-280B/G Shielded are lightweight transportable shelters designed for use with the Area Type Communication Systems and other communication systems.

1-2. Maintenance Forms and Records. Department of the Army forms and procedures used for equipment maintenance will be those prescribed by DA Pam 738-750, The Army Maintenance Management System (TAMMS).

1-3. Reporting Equipment Improvement Recommendations (EIRs). If your Shelter needs improvement, let us know. Send us an EIR. You, the user, are the only one who can tell us what you don't like about your equipment. Let us know why you don't like the design or performance. Put it on an SF 368 (Product Quality Deficiency Report). Mail it to: Commander, S Army Aviation and Troop Command, ATTN: AMSAT-I-MDO, 4300 Goodfellow Blvd., ST. Louis, MO 63120-1798. We'll send you a reply.

1-4. Destruction of Army Materiel to Prevent Enemy Use. Destruction of Army equipment to prevent enemy use shall be in accordance with TM 750-244-3.

1-5. **Preparation for Shipment and Storage.** Refer to paragraphs 3-21 through 3-24 for shipment and storage preparation data.

1-6. **List of Abbreviations.**

RFI	Radio Frequency Interference
EMI	Electromagnetic Interference
TMDE	Test, Measurement and Diagnostic Equipment
CARC	Chemical Agent Resistive Coating

Section II. EQUIPMENT DESCRIPTION


Subject	Para	Page
Equipment Characteristics, Capabilities and Features	1-7	1-2
Location and Description of Major Components	1-8	1-2
Differences Between Models	1-9	1-3
Equipment Data	1-10	1-3
Shelter Marking	1-11	1-3
Safety, Care and Handling	1-12	1-3

1-7. **Equipment Characteristics, Capabilities and Features.** The S-280B/G and S-280B/G Shielded shelters are lightweight, relocatable shelters used to transport and house ground communications equipment. The foam and beam shelter construction consists of aluminum face sheets enclosing a polyurethane foam composition core. The shielded shelters are equipped with radio frequency/electromagnetic interference (RFI/EMI) shielding to protect the electronic equipment contained inside. The shield is a continuous metallic surface which includes the shelter panel inner face sheets and conductive materials which maintain continuity around joints, door openings and other possible sources of radiation leakage. Shielded shelters also have an RFI/EMI filter inside the emergency exit panel. Shielded shelters can be identified by the metallic door gasket which mates with another conductive surface on the doorjamb. The shelter is designed for outdoor use in all weather conditions.

1-8. **Location and Description of Major Components.** (figure 1-1)

ITEM	DESCRIPTION
1. Door Assembly	Provides access to equipment contained in shelter.
2. Emergency exit panel	Contains air vent and filter and serves as an emergency exit. In shielded shelters, inner door also houses RFI/EMI filter.
3. Lifting eye assemblies	Provide hookup points for sling assembly when lifting shelter and when securing shelter onto truck.
4. Towing eye assemblies	Provide hookup points for guide rope when guiding sling-lifted shelter into position.
5. Roof Access Steps	Allow access to roof.

1-9. **Differences Between Models.** The S-280B/G Shielded shelter (NSN 5411-00-001-4093) differs from the S-280B/G (NSN 5411-00-117-2868) only in its radio frequency/electromagnetic suppression capabilities. Components of RFI/EMI shielding are described in paragraph 1-7.

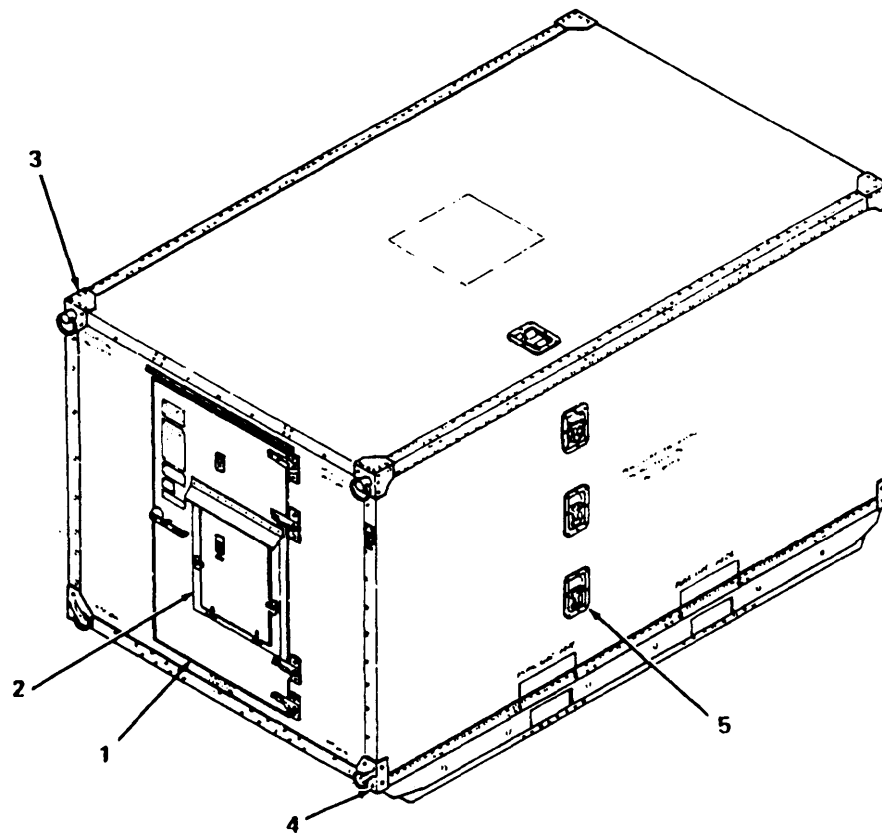

4753-002


Figure 1-1. Major Shelter Components.

1-10. Equipment Data.

Height	83.325 in. (21 1.65 cm)
Width	87 in. (220.98 cm)
Length	147 in. (373.68 cm)
Gross weight	1380 lb (627 kg)
Cubage	617 ft ³ (17.47 m ³)
Load on skids	0.9 psi

1-11. **Shelter Marking.** Shelter markings are shown in figure 1-2. Lettering is stenciled or silkscreened in accordance with MIL-M-1321 GR II. The color used is black, MIL-C-46168.

1-12. **Safety, Care and Handling.** Throughout this manual are warnings, cautions and notes designed to protect personnel and equipment when handling the shelter. Learn the warnings on the warning page before attempting to perform maintenance on the shelter, and observe all warnings, cautions and notes as you come upon them in the text.

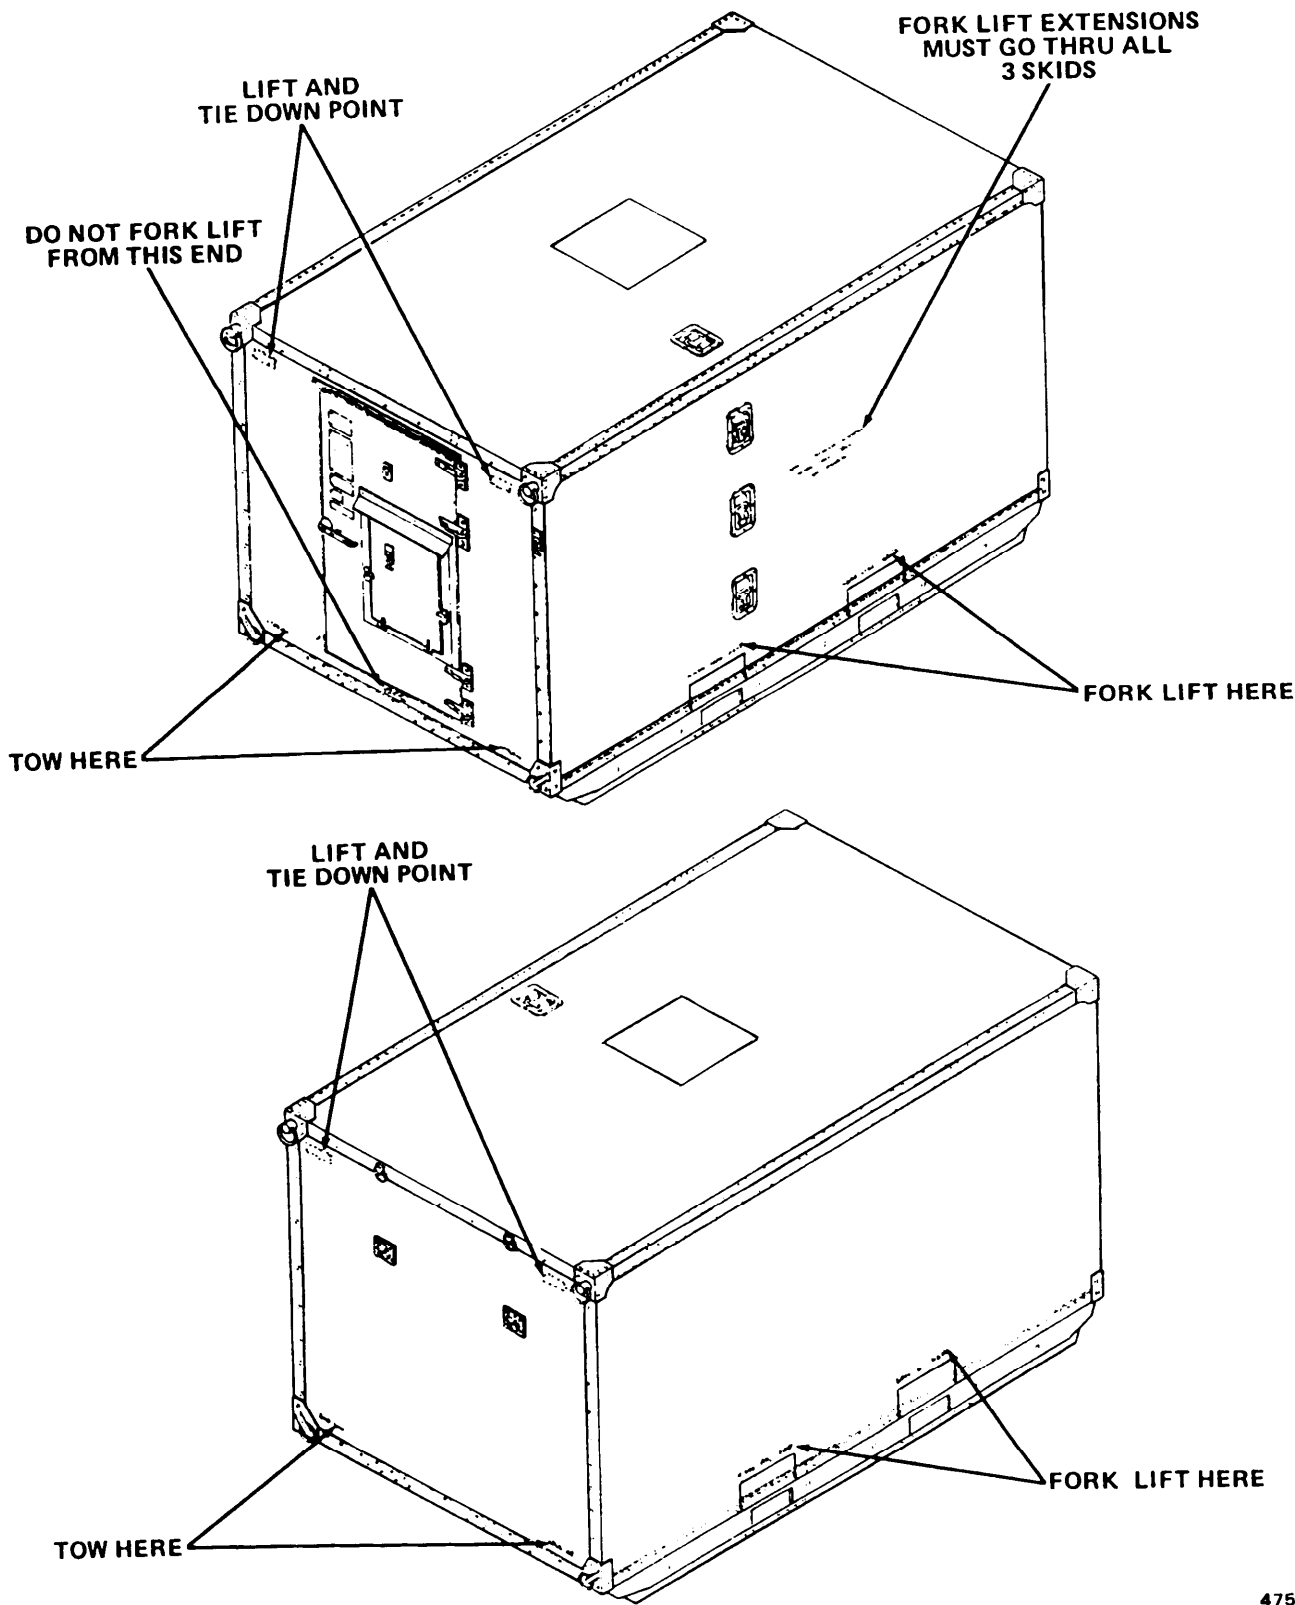

4753-003

Figure 1-2. Shelter Marking.

CHAPTER 2

OPERATING INSTRUCTIONS

Subject	Section	Page
Operator Preventive Maintenance Checks and Services (PMCS)	I	2-1
Operation Under Usual Conditions	II	2-4
Operation Under Unusual Conditions	III	2-6

Section I. OPERATOR PREVENTIVE MAINTENANCE CHECKS AND SERVICES (PMCS)

Subject	Para	Page
General	2-1	2-1
Explanation of Columns	2-2	2-1

2-1. **General.** Your Preventive Maintenance Checks and Services table lists the inspections required to keep your equipment in good operating condition.

a. Before You Operate. Always keep in mind the CAUTIONS and WARNINGS. Perform your before (B) PMCS.

b. While You Operate. Always keep in mind the CAUTIONS and WARNINGS. Perform your during (D) PMCS.

c. After You Operate. Be sure to perform your after (A) PMCS.

d. Weekly. (Perform your weekly (W) PMCS.

e. Once Each Month. Perform your monthly (M) PMCS.

f. If Your Equipment Fails to Operate. If your equipment does not perform as required, notify higher level of maintenance. Report any malfunctions or failures on the proper DA Form 2404 or refer to DA Pam 738-750.

2-2. Explanation of Columns.

a. Item Number. The item number is to be used as a source number for the TM number column on DA Form 2404, Equipment Inspection and Maintenance Worksheet, when recording PMCS results.

b. Interval. The interval column of your PMCS table tells you when to do a certain check or service.

c. Item To Be Inspected. This column lists the components that require inspection.

d. Procedures. This column lists the faults to check for and procedures to follow.

e. Equipment is Not Ready/Available If. This column tells you when and why your equipment cannot be used.

2-2. Explanation of Columns (cont).

NOTE

Perform your weekly as well as before checks if you are the assigned operator and have not operated the equipment since the last weekly check, or if you are operating the equipment for the first time.

Table 2-1. Operator Preventive Maintenance Checks and Services.

NOTE

Within the designated interval, these checks are to be performed in the order listed.

B – Before						D – During						A–After						W – Weekly						M – Monthly						
Item No.	Interval					Item to be Inspected	Procedures Check for and have repaired or adjusted as necessary												Item is Not Ready/ Available If:											
	B	D	A	W	M																									
1	•			•		Door Handle	Make sure handle operates smoothly without binding or jamming.												Door cannot be opened or cannot be closed securely.											
2	•			•		Emergency Exit Panel	a. Make sure cover can be held in the open position using T-latch. b. Make sure weather gasket is in good condition.																							
3	•			•		Door Brace Assembly	Make sure door brace assembly pivot points rotate easily. Check for loose or missing hardware.																							
4	•			•		Door Assembly	a. Make sure door opens and closes smoothly without binding. Check hinges for rust, loose or missing hardware. Lubricate hinges. b. Make sure drip cap and drip molding are intact. c. Make sure air filters and louvers are not missing or blocked.																							
																			c. Air filters or louvers are missing or blocked.											

Table 2-1. Operator Preventive Maintenance Checks and Services (cont).

						B – Before	D – During	A – After	W – Weekly	M – Monthly
Item No.	Interval									
	B	D	A	W	M	Item to be Inspected	Procedures Check for and have repaired or adjusted as necessary			Item is Not Ready/ Available If:
4						Door Assembly (cont)	d. Check door surfaces for punctures. e. Make sure weather gaskets are in good condition.			
5	•				•	Lifting and Towing Eye Assemblies	a. Inspect for excessive wear. b. Inspect for rust, loose or missing hardware. c. Make sure rings and pins rotate freely.			
6					•	Roof Access Steps	a. Make sure steps stay in up or down position as required. b. Check for loose or missing hardware.			
7					•	Roof Handle	Check for loose or missing hardware.			
8		•				Drain Plug	Make sure drain plug is in place.			Drain plug is missing (shielded shelters).
9		•			•	RFI/EMI Components (S-280B/G Shielded)	a. Inspect metal door gaskets. b. Inspect filter. c. Check for presence of drain plug washer, keeper shims and hinge shims.			a. One or both gaskets are missing or damaged. b. Filter is damaged or missing. c. A washer or shim is missing.
10	•				•	Wall, Floor and Ceiling Panels	Inspect for punctures and delamination.			Punctures are present.

Table 2-1. Operator Preventive Maintenance Checks and Services (cont).

B – Before		D – During		A – After		W – Weekly		M - Monthly	
Item No.	Interval					Item to be Inspected	Procedures Check for and have repaired or adjusted as necessary	Item is Not Ready/ Available If:	
	B	D	A	W	M				
11	●				●	Skids and Mounting Brackets	Make sure skids and mounting brackets are securely mounted to shelter and are undamaged.		

Section II. OPERATION UNDER USUAL CONDITIONS

Subject	Para	Page
Assembly and Preparation for Use	2-3	2-4
Initial Adjustments	2-4	2-4
Operator Procedure	2-5	2-4
preparation for Movement	2-6	2-4
Instruction and Warning Plates	2-7	2-5

2-3. **Assembly and Preparation for Use.** There are no assembly or preparation procedures that must be performed before using the basic shelter. For all assembly and preparation procedures applicable to a configured shelter, refer to the end item technical manual.


2-4. **Initial Adjustments.** The shelter itself requires no adjusting. However, the operator must make certain the shelter is positioned so that the doors can be fully opened and closed and that any external equipment required for operation of the shelter-contained equipment can be properly installed. Refer to the end item technical manual for additional procedures applicable to the configured shelter.

2-5. **Operating Procedures.** There are no operating procedures applicable to the basic shelter. Refer to the end item technical manual for operating procedures applicable to the configured shelter.

2-6. **Preparation for Movement.** Before moving the shelter, make sure the doors are closed and padlocked. If the shelter is being moved by truck, make sure the shelter is properly tied down and blocked to prevent movement. Refer to paragraph 3-5 for instructions for securing the shelter on a truck. If the shelter must be loaded onto a truck for movement, refer to paragraph 3-5 for lifting and loading instructions. Refer to the end item technical manual for additional preparation instructions applicable to the configured shelter.

2-7. Instruction Plates. (figure 2-1)

ITEM	CONTENT
1. Airborne Instruction Plate	Open cover before airlift Keep vent cover open when shelter is occupied Keep drain plug loose during air and rail transport
2. Paint Instruction Plate	The surfaces of this shelter have been painted with CARC For touch-up Exterior – Use only lusterless green 383 polyurethane IAW MIL-C-46168 Interior – Use only epoxy polyamide IAW MIL-C-22750
3. Secondary Exit Data Plate	Secondary exit Remove 4 hand knobs Lift out exit panel
4. Door Closing Instruction Plate	Push catch to release door stop brace.

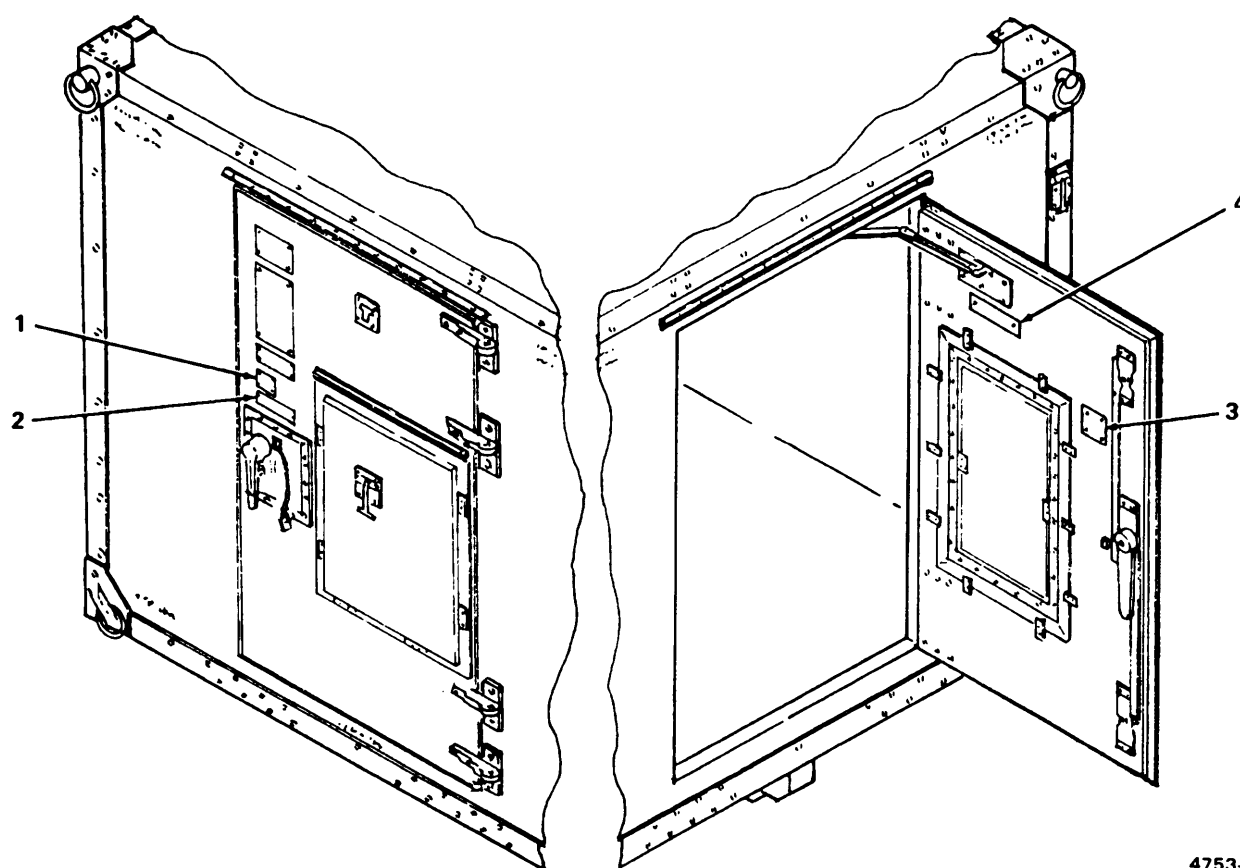

4753-004

Figure 2-1. Instruction and Warning Plates.

Section III. OPERATION UNDER UNUSUAL CONDITIONS

Subject	Para	Page
Operation in Unusual Weather	2-8	2-6
Emergency Procedures	2-9	2-6

2-8. **Operation In Unusual Weather.** The shelters are designed for use in all weather. However, shelters located at coastal sites and subject to salt air deterioration, or areas subject to wind-driven sand or coral dust shall be inspected by site personnel at least once every week to assure timely determination of maintenance and repair needs. Additional requirements for operation in unusual weather can be found in the end item technical manual.

2-9. **Emergency Procedures.** Any damage to the shelter walls or ceiling must be patched immediately to prevent water intrusion. In an emergency, any kind of tape or water-resistant materials may be used to cover a puncture or a large hole. Temporary patches must be replaced with permanent patches as soon as possible. In a shielded shelter, temporary patches must be replaced as soon as possible to restore RFI/EMI suppression.

CHAPTER 3

UNIT MAINTENANCE INSTRUCTIONS

Subject	Section	Page
Lubrication	I	3-1
Repair Parts, Special Tools, TMDE and Support Equipment	II	3-1
Service Upon Receipt	III	3-1
Troubleshooting	IV	3-4
Unit Maintenance Procedures	V	3-7
Preparation for Shipment and Storage	VI	3-35

Section I. LUBRICATION

3-1. **Lubrication Instructions.** There is no scheduled lubrication. However, lubricate door and emergency exit panel cover hinges, latches and locking mechanisms, door brace assembly, roof access steps and lifting and towing eye assemblies to prevent rust and corrosion. Check these parts frequently to be sure they are adequately lubricated. Lubricate with Solid Film Lubrican, MIL-L-23398. There is no scheduled lubrication for the shelter. Lubricate as necessary to prevent rust corrosion and wear.

Section II. REPAIR PARTS, SPECIAL TOOLS, TMDE AND SUPPORT EQUIPMENT

Subject	Para	Page
Common Tools	3-2	3-1
Special Tools, TMDE and Support Equipment	3-3	3-1
Repair Parts	3-4	3-1

3-2. **Common Tools.** A complete list of common tools and tool kits is given in Section III of Appendix B, Maintenance Allocation.

3-3. **Special Tools, TMDE and Support Equipment.** There are no special tools or equipment needed to maintain the shelters.

3-4. **Repair Parts.** Repair parts for unit maintenance of the shelters are listed and illustrated in TM 10-541 1-206-24P.

Section III. SERVICE UPON RECEIPT

Subject	Para	Page
Service Upon Receipt of Materiel	3-5	3-2
Site Requirements	3-6	3-4

3-5. **Service Upon Receipt of Materiel.** Inspect the shelter for damage incurred during shipment. If the shelter has been damaged, report the damage on SF 364, Report of Item Discrepancy. If the drain plug has been loosened for shipment, tighten it. If the shelter is crated or pallet-mounted, refer to the end item technical manual for unpacking instructions. If it is necessary for the shelter to be loaded onto a truck or transferred from one truck to another, lift, pad and secure the shelter as follows:

WARNING

If shelter panel is punctured during loading or securing, repair puncture as soon as possible to prevent moisture from seeping into panels, and to restore RFI/EMI shielding in shelters having this requirement. Failure to do so may result in exposure of personnel to radiation.

a. *Lifting Shelter.* (figure 3-1)

CAUTION

On "Craig Round Corner" shelters, do not attempt to lift shelter with sling assembly cables connected to tiedown eyes. Damage to equipment may result.

- (1) Attach sling assembly to all four lifting rings on shelter so that turnbuckle ends of cables are next to lifting rings. Be sure to use correct sling assembly (hold down assembly). (See Appendix C.)
- (2) Place sling assembly on top of shelter.
- (3) Connect four sling hooks at opposite ends of cables to sling assembly lifting ring.
- (4) Insert lifting hook of lifting device (crane or helicopter) into lifting ring.
- (5) Tie a 1/2-inch rope, at least 15 feet long, to each rear towing eye.

CAUTION


Do not jerk, bounce or jar shelter when lifting. Avoid swinging shelter from side to side. Do not attempt to butt or push shelter into place with a forklift. If shelter is crated, pallet-mounted or has forklift instructions stenciled on exterior, a forklift may be used to move shelter in accordance with instructions.

- (6) Slowly lift shelter with crane or helicopter.

b. *Loading Shelter onto Truck.* (figure 3-1)

WARNING

To avoid injury to personnel and damage to shelter, only personnel actually engaged in loading operation should be permitted near truck, lifting device and shelter. To eliminate confusion, all instructions must come from loading crew supervisor.

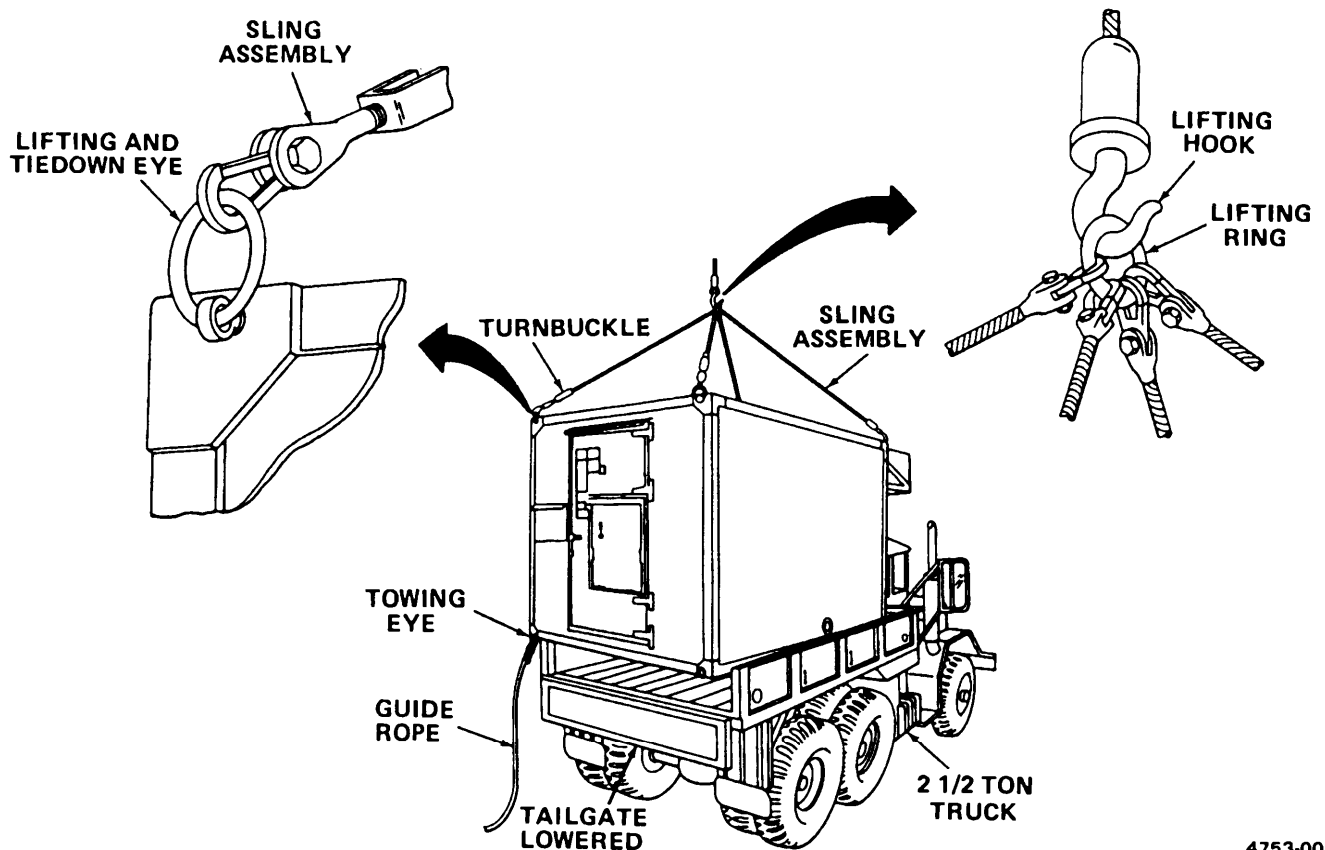

4753-005

Figure 3-1. Lifting and Loading Shelter.

NOTE

Some procedures require the addition of dunnage to truck bed or the attachment of tiedown eyes to truck before loading shelter onto truck. Refer to technical manual for type of truck being used.

- (1) Lower truck tailgate and make sure all tools and equipment have been removed from truck bed.
- (2) Position one person at free end of each rope to guide shelter into place.
- (3) Lift shelter to a position high enough to clear truck bed.
- (4) Back truck into position under shelter.

WARNING

To avoid injury to personnel, all personnel must remain clear of truck while shelter is being lowered into place.

- (5) With one person at each rope, guide shelter into position so that it is aligned above truck bed, and maintain that position while lowering shelter into place on truck bed.

3-5. Service Upon Receipt of Materiel (cont).

- (6) Remove lifting ring from lifting hook and separate lifting ring from sling hooks. Remove sling hooks from lifting eyes and remove ropes from rear towing eyes.

c. *Securing shelter on Truck.* (figure 3-2)

- (1) Install plate and eye bolt assemblies (part of sling assembly) on cargo bed siderails of truck as shown in figure 3-2.
- (2) Hook ends of four sling assemblies to tiedown eyes at each top corner of shelter, using hooks at furthest end of cables from turnbuckles.
- (3) Hook sling hooks at opposite end of cables to appropriate eye bolts on truck. Make sure sling hooks point away from shelter.
- (4) Tighten all turnbuckles evenly by hand. Then turn each turnbuckle an additional one-half turn with a bar or rod inserted in turnbuckle slot.

CAUTION


Do not overtighten turnbuckles. Overtightening may tear lifting and tiedown eyes from shelter or damage eye assembly or shelter.

- (5) Insert appropriate size wooden blocks between shelter skids and sides of truck bed to prevent sideways movement strain on sling cables.
- (6) Insert appropriate size wooden blocks between shelter skids and cab wall of bed to protect cab wall and shelter towing eyes.
- (7) Raise and secure truck tailgate.

3-6. **Site Requirements.** Site requirements will depend on the requirements of the equipment contained in the shelter. Refer to the end item technical manual for siting instructions.

Section IV. TROUBLESHOOTING

3-7. **Troubleshooting.** This section contains troubleshooting information for malfunctions which may develop in the shelters. Fault isolation is limited to those components which maybe repaired or replaced at the unit level. Table 3-1 lists the common malfunctions you may encounter during operation or maintenance of the shelter. Each malfunction is followed by a list of tests or inspections and corrective actions. These tests or inspections and corrective actions should be performed in the order listed. This manual cannot list all malfunctions that may occur. If you encounter a malfunction that is not listed or that cannot be corrected by the listed corrective actions, notify your supervisor.

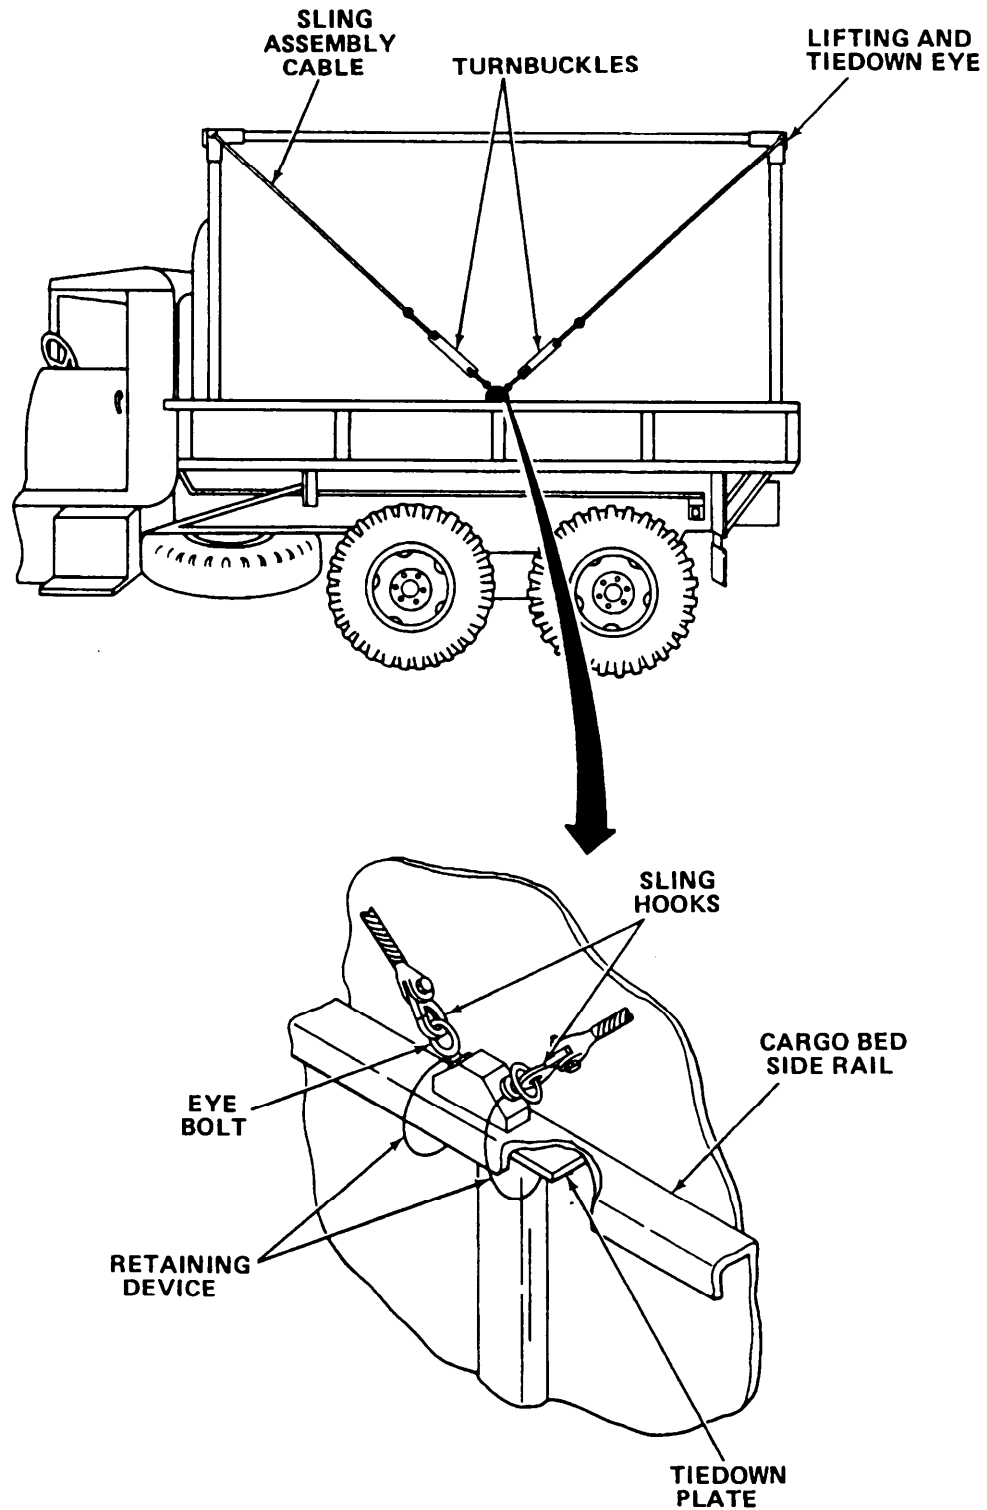

4753-006

Figure 3-2. Securing Shelter on 2 1/2 Ton Truck.

Table 3-1. Troubleshooting

MALFUNCTION	TEST OR INSPECTION	CORRECTIVE ACTION
1. DOOR DOES NOT OPEN OR CLOSE SMOOTHLY		
	Step 1. Inspect hinges for inadequate lubrication.	Lubricate as required (para 3-1).
	Step 2. Notify higher level of maintenance.	
2. DOOR DOES NOT STAY OPEN		
	Step 1. Check to see if door brace catch is missing or improperly installed.	Install catch (para 3-11).
	Step 2. Check to see if door brace assembly is detached from door or door stop angle.	Replace missing hardware (para 3-11).
3. DOOR HANDLE IS JAMMED OR DOES NOT OPERATE SMOOTHLY		
	Step 1. Inspect components for inadequate lubrication.	Lubricate as required (para 3-1).
	Step 2. Inspect door handle and latching mechanism for missing or damaged components.	Repair or replace components as required (para 3-15).
4. WATER IS GETTING INTO SHELTER		
	Step 1. Inspect shelter walls and ceiling for punctures.	Patch any holes (para 3-9.c).
	Step 2. Check to see if roof access steps or d-ring hand holds have pulled away from shelter wall.	Apply sealer to gaps around step flange, or replace step (para 3-17) or d-ring (para 3-18).
	Step 3. Notify higher level of maintenance.	

Table 3-1. Troubleshooting (cont).

MALFUNCTION	TEST OR INSPECTION	CORRECTIVE ACTION
5. THERE IS EVIDENCE OF RADIO FREQUENCY/ELECTROMAGNETIC INTERFERENCE (S-280 B/G SHIELDED)		
	Step 1. Check for missing latch keeper shims.	Install shims (para 3-15).
	Step 2. Check for missing drain plug washer.	Install washer (para 3-19).
	Step 3. Notify higher level of maintenance.	

Section V. UNIT MAINTENANCE PROCEDURES

Subject	Para	Page
General	3-8	3-7
General Repair Procedures	3-9	3-8
Touchup Painting	3-10	3-17
Door Brace Assembly	3-11	3-18
Door Assembly	3-12	3-21
Emergency Exit Panel Assembly	3-13	3-22
T-Latches and Holders	3-14	3-23
Door Latch Assembly	3-15	3-24
Air inlet Filter	3-16	3-30
Recessed Step Pan Assemblies	3-17	3-31
D-Ring Assemblies (Hand Holds)	3-18	3-32
Drain Plug and EMI Washer	3-19	3-34
RFI/EMI Components	3-20	3-35

3-8. General. This section contains maintenance procedures which are the responsibility of unit maintenance, as authorized by the Maintenance Allocation Chart (appendix B). Since most shelters contain sensitive electronic equipment that cannot be easily removed, unit level maintenance and repair will primarily involve shelter exteriors or easily accessible interior areas, unless floors, ceilings or walls have evidence of water intrusion which can jeopardize operation of the equipment. The shelters shall be returned to the depot for repair if any of the following conditions exist:

- a. Panel damage spans a structural member.
- b. Replacement of an entire wall, ceiling or floor is required.
- c. Extensive equipment removal beyond the capability of the using unit is required.

3-8. General (cont).

d. Welding is required.

e. Damage to a structural member is severe enough to cause distortion of a wall, especially in edge or corner areas.

f. Lift, tow or tiedown fittings or corner castings are damaged severely enough to indicate possible damage to the underlying structural member.

NOTE

If nature of damage warrants it, print a caution notice using 4-inch high letters on all outside walls of the shelter as follows: CAUTION: DAMAGED SHELTER. DO NOT SLING LIFT.

Coat threads of all screws and bolts with sealer before installing. Fill rivet and rivnut holes with sealer before using.

Unless otherwise noted, procedures described apply to all three configurations of shelter covered by this technical manual.

Unless otherwise noted, all procedures can be performed by one person, using standard tools listed in Appendix B, Section III.

3-9. General Repair Procedures. The procedures described in this paragraph are general procedures that may be needed during repair or replacement of many of the shelter components. Wherever these general procedures apply, they are referenced at the appropriate point in the specific maintenance procedure paragraph.

a. Blind Rivet Installation and Removal. Blind rivets are used in locations where only one side of the area to be worked on is accessible. Blind pop rivets must be used in the shelter foam and beam panels, since the hammering required to install conventional rivets would damage the material. The types of rivets used in the shelter are shown in figure 3-3 and described in table 3-2. When installing floor patches, countersunk head rivets are preferred. Dome head rivets are an acceptable alternate. When installing interior wall patches, countersunk head rivets shall be used in any location in which dome head rivets will interfere with the proper installation of equipment. Closed end rivets shall be used for exterior repairs and floor repairs to prevent moisture and dirt from entering panels.

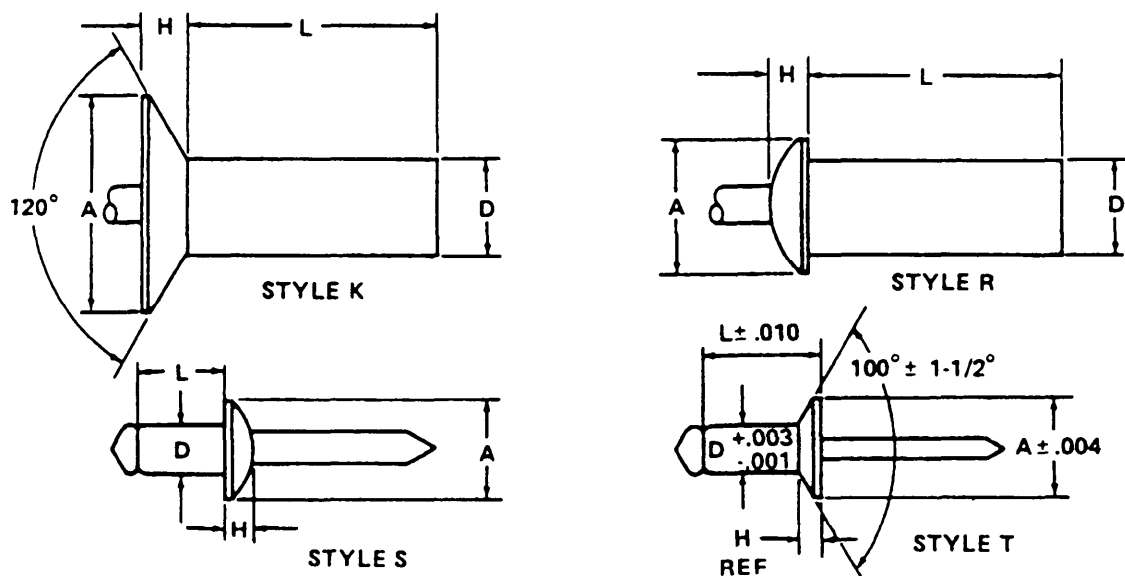


Figure 3-3. Rivet Types.

Table 3-2. Blind Rivets.

Dash No.	Part No.	Style	Dim A	Dim H	Dim D	Dim L
SC-D-200131-29	AD62H	R	0.375	0.066	3/16	0.325
SC-D-200131-31	AD43H	R	0.236	0.036	1/8	0.357
SC-D-200131-35	AK64H	K	0.375	0.060	3/16	0.450
SC-D-200131-33	AD64H	R	0.375	0.066	3/16	0.450
SC-D-200131-30	AD42H	R	0.236	0.036	1/8	0.295
SC-D-200131-32	AD66H	R	0.375	0.066	3/16	0.575
SC-D-200131-26	AD45H	R	0.236	0.036	1/8	0.482
SC-D-200131-25	AD44H	R	0.236	0.036	1/8	0.420
SM-D-555530-7						
SC-D-200131-19	OSR-8D					
SC-D-200131-34	AD63H	R				
	MS20600AD4W-2	S	0.250	0.054	0.125	0.232
	NAS1398D6-5					
	NAS1399D8-5					
	NAS1399D4-4					
	NAS1399D4-3					
	NAS1398D4-4					
	NAS1739E4-3					
	MS20426AD6-8	K	0.353	0.070	0.187	0.500
	MS20470AD6-8	R	0.375	0.080	0.187	0.500
	MS20600AD6W-2	S	0.375	0.080	0.187	0.277
	MS20600AD6W-3	S	0.375	0.080	0.187	0.340
	MS20600AD6W-4	S	0.375	0.080	0.187	0.402
	MS20600AD6W-5	S	0.375	0.080	0.187	0.465

Table 3-2. Blind Rivets (cont).

Dash No.	Part No.	Style	Dim A	Dim H	Dim D	Dim L
SC-D-200131-4 SM-D-555530-5 SM-D-555530-6	MS20600AD8W-3	S	0.500	0.107	0.250	0.447
	MS20600AD8W-4	S	0.500	0.107	0.250	0.385
	MS20600AD4W-3	S	0.250	0.054	0.125	0.295
	OSR-8C					
	9SPB-RB-5					
	0SR-8B					
	MS20601AD6W-6	T	0.353	0.070	0.187	0.527
	MS20601AD6W-5	T	0.353	0.070	0.187	0.465
	MS20600AD4W-4	S	0.250	0.054	0.125	0.357
	MS20600AD8W-5	S	0.500	0.107	0.250	0.510
	MS20600AD8W-6	S	0.500	0.107	0.250	0.572
	MS20601AD6W-3	T	0.353	0.070	0.187	0.340
	MS20601AD6W-2	T	0.353	0.070	0.187	0.277
	MS20600AD6-6	S	0.375	0.080	0.187	1.200
	MS20601AD4W-3	T	0.225	0.042	0.125	0.750
	MS20601AD5W-3	T	0.286	0.055	0.156	0.808
	MS20601AD5W-2	T	0.286	0.055	0.156	0.620

Rivet Body Material _____
A = Aluminum

Head Style _____
D = Dome head
K = Countersunk

Rivet Diameter in 32nds of an Inch _____
Example: 4 = 4/32 or 1/8 inch
body diameter

Max. Grip in 16ths of an Inch _____
Example: 4 = 4/16 or 1/4 inch
maximum grip range

Mandrel Material _____
A = Aluminum
No letter= Carbon steel

Core Design _____
H = Hollow Core
S = Solid core

4 4 A H
↑ ↑ ↑ ↑

(1) *Installation.* (figure 3-4)

NOTE

When installing new rivet in same location as a rivet that has been removed, if diameter of hole in structure has been enlarged during removal of rivet, use next larger diameter rivet for replacement.

Clean rivets with solvent before installing.

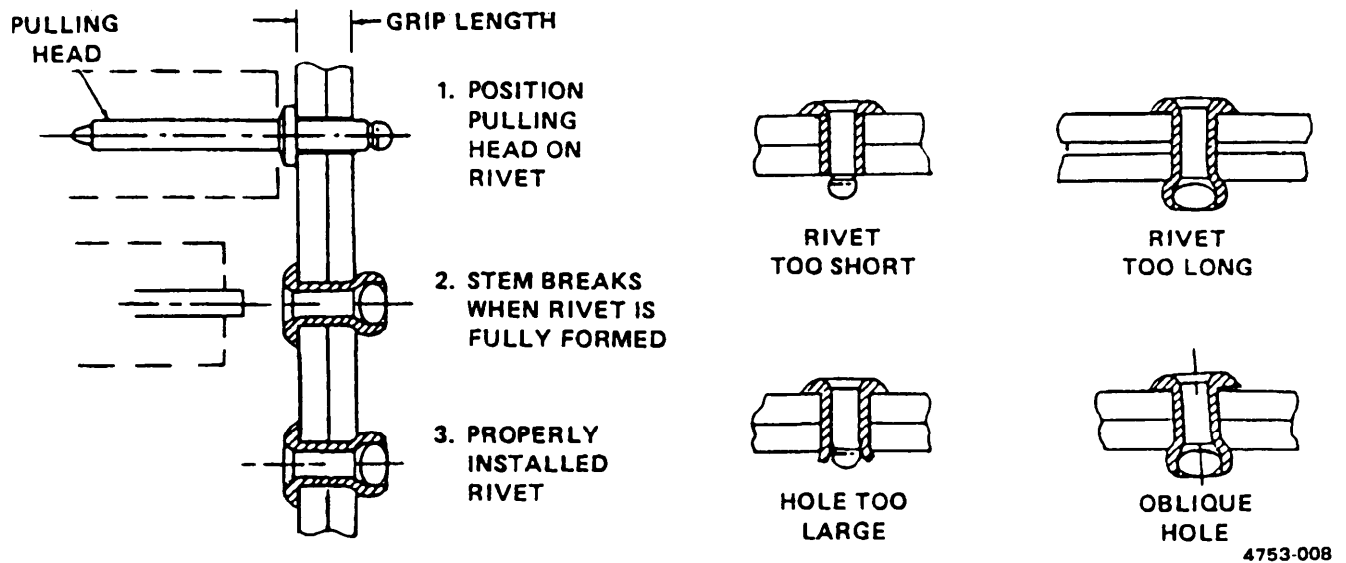


Figure 3-4. Installing Blind Rivets.

- (a) Determine type, size and grip range of rivet to be used. Grip length equals combined thickness of materials being riveted together. Grip range of rivet must encompass grip length.

WARNING

Drilling creates metal chips which may enter eyes and cause serious injury. Eye protection is required.

NOTE

Drill hole size must match size of rivet being used.

Quantities of sheets maybe drilled at the same time when held together with sheet fasteners.

- (b) Drill hole in structure.

- (c) Remove all metal chips and remove burrs from drilled holes.

3-9. General Repair Procedures (cont).

- (d) If flush head rivet is being installed, countersink hole using a 100-degree machine countersink.

NOTE

Coat all rivets with sealer before installing.

- (e) Insert rivet in hole. Make sure sheets are held tightly together before upsetting or pulling rivet.
- (f) Select proper pulling head for rivet being installed and install pulling head on rivet gun.
- (g) Insert stem of rivet into pulling head.
- (h) With pulling head parallel to axis of rivet, upset rivet. Exert firm pressure but do not bend or buckle metal sheets. Stem will break off below rivet head surface. No trimming should be required.
- (i) Make sure riveted parts are not loose, rivet does not rotate and rivet head is seated tightly against riveted surface. If rivet is loose or improperly installed, remove it and install a new one.

- (2) *Removal.* (figure 3-5)

WARNING

Drilling creates metal chips which may enter eyes and cause serious injury. Eye protection is required.


NOTE

When drilling through rivet head, be careful to avoid enlarging hole in structure. Keep drill perpendicular to material being drilled and do not exert excessive pressure on drill, Or replacement rivets will be too loose.

- (a) Drill through head of rivet only, using hole in rivet as a guide. Use proper drill size as follows:

Rivet size (in.)	Drill size
1/8	No. 31
5/32	No. 21
3/16	No. 12
1/4	1/4 inch


- (b) Using a pin punch, pry off rivet head.
- (c) Using pin punch, push out remainder of rivet shank. If shank will not easily push out, drill it out.

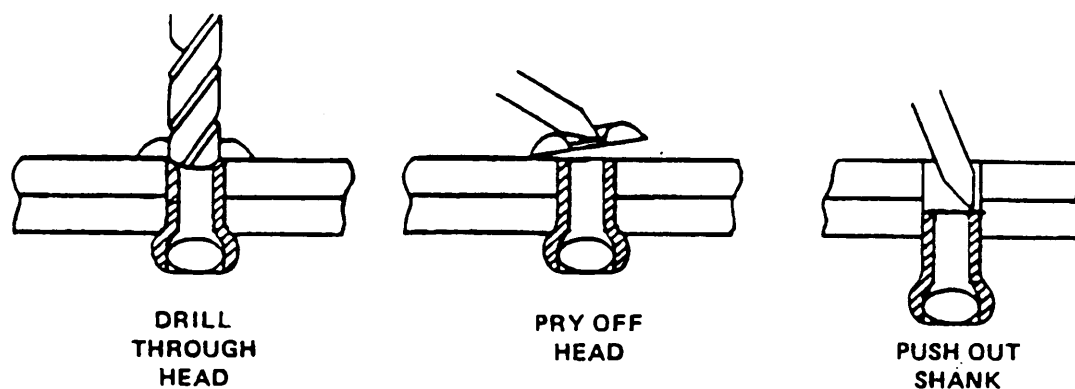

4753-009

Figure 3-5. Removing Blind Rivets.

b. Rivnut Installation and Removal. Rivnuts (threaded inserts) are tubular rivets with internal threads and are used throughout the shelter wherever blind threads are required. The types of rivnuts used in the shelter are shown in figure 3-6 and described in table 3-3. Flat head rivnuts may be used wherever head thickness will not interfere with installation of equipment. Countersunk head rivnuts are used for flush installation. Keyed rivnuts are used in locations which are subject to vibration and torque. Closed end rivnuts must be used for exterior repairs and floor repairs to keep moisture and dirt from entering panels. Open end rivnuts may be used in areas where sealing is not required.

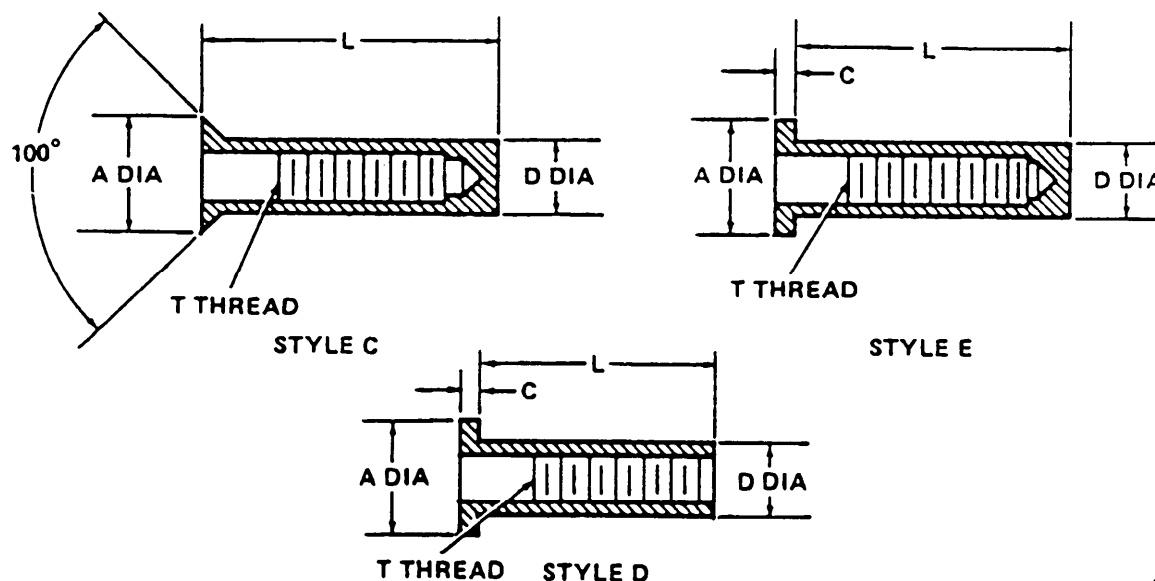

4753-010

Figure 3-6. Rivnuts (Threaded Inserts).

3-9. General Repair Procedures (cont).


Table 3-3. Rivnuts.

Dash No.	Part No.	Style	Dim A	Dim D	Dim L	T	Dim C	Grip Range
SM-D-555530-10	S25B211	C	0.529	0.332	1.062	1/4-20 UNC-3B		.151 -.211
SC-D-200131-7	S25B211	C	0.529	0.332	1.062	1/4-20 UNC-3B		.151 -.211
SM-D-555530-15	S31B500							
SC-D-200131-8	S31B500							
SC-D-200131-22	S25B140	E	0.475	0.332	1.000	1/4-20 UNC-3B	0.058	.080 -.140
SM-D-555530-20	S37B115							
SC-D-200131-9	S37B115							
SM-D-555530-21	S37B285							
SC-D-200131-10	S37B285							
SM-D-555530-24	S31B275							
SC-D-200131-11	S31B275							
SC-D-200131-20	S10B216							
SC-D-200131-21	S8B120							
SC-D-200131-24	S10B130							

(1) Installation. (figure 3-7)

NOTE

When installing new rivnut in same location as rivnut that has been removed, if diameter of hole in structure has been enlarged during removal, use next larger diameter rivnut for replacement.

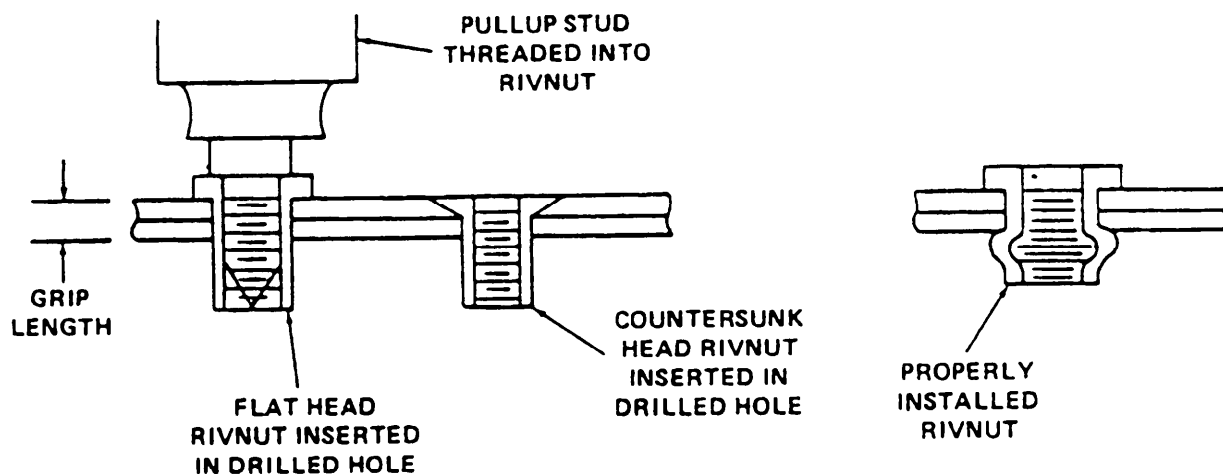

4753-011

Figure 3-7. Installing Rivnuts.

- (a) Determine thread size, grip range, style and material of rivnut to be used. Grip length equals combined thickness of materials being fastened together. Grip range of rivnuts must encompass grip length.

WARNING

Drilling creates metal chips which may enter eyes and cause serious injury. Eye protection is required.

NOTE

Drill hole size must match size of rivnut being installed. Quantities of sheets maybe drilled at the same time when held together with sheet fasteners.

- (b) Drill hole in structure.
- (c) Remove all metal chips and remove burrs from drilled holes.
- (d) If a countersunk head rivnut is being installed, countersink hole using a 100-degree machine countersink.

NOTE

Coat rivnut with sealer before installing.


- (e) Insert rivnut in hole. Make sure sheets are held tightly together before pulling.
 - (f) Thread stem of a pullup stud into rivnut.
 - (g) With pullup stud parallel to axis of rivnut, pull upon rivnut. Exert firm pressure but do not bend or buckle metal sheets.
 - (h) Make sure fastened parts are not loose, rivnut does not rotate and rivnut head is seated tightly against surface. Make sure rivnut threads are in good condition. If threads are damaged or rivnut is improperly installed, remove it and install a new one.
- (2) *Removal.* (figure 3-8)

WARNING

Drilling creates metal chips which may enter eyes and cause serious injury. Eye protection is required.

- (a) Drill through head of rivnut, using same size drill used to make original hole. Counterbore in rivnut will act as a drill guide.
- (b) Remove head of rivnut.

3-9. General Repair Procedures (cont).

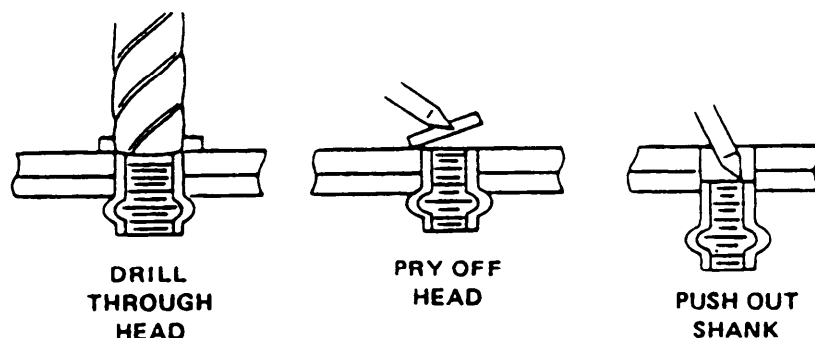

4753-012

Figure 3-8. Removing Rivnuts.

CAUTION

Do not puncture opposite face sheet of panel when punching out rivnut shank.

- (c) Punch out shank of rivnut, using a pin punch slightly smaller than hole in structure. Punch only enough to disengage. Move rivnut aside to install new rivnut.

c. Temporary Panel Repair. Any puncture in the shelter exterior, including punctures in the door skin, must be patched immediately to prevent water intrusion. In shelters with RFI/EMI shielding, any rupture of the future sheet must be patched immediately to prevent radiation leakage. Dents without pictures do not require patching. However, if bare metal is exposed, touchup paint shall be applied (para 3-10).

Materials/Parts:	Adhesive (items 2,3,4 or 5, Appendix D)	Sandpaper, grit nos. 40,60 and 80 (Items 26,27 and 28, Appendix D)
	Tape, pressure sensitive (Item 35, Appendix D)	Clean Cloths (Item 9 or 10, Appendix D)
	Electrically conductive tape (for shielded shelters) (Item 32, Appendix D)	Solvent (item 37, Appendix D)
		Gloves (Item 12, Appendix D)
		Goggles (item 38, Appendix D)

CAUTION

Paint strippers can contaminate panel core, adhesive and sealers. Do not use paint strippers to remove paint.

RFI/EMI shielded shelters should not be used until an RFI/EMI suppression patch has been applied.

NOTE

Ceiling panel composition is the same as wall panel composition. The same method of repair applies to walls and ceilings.

- (1) Bend edges of puncture in below surface of unbroken face sheet. Do not allow broken edges to contact opposite face sheet.
- (2) Remove loose fragments of foam and dust.

WARNING

Solvents are flammable and toxic. Keep away from heat and open flames. Use in a well-ventilated area. Avoid skin and eye contact and breathing of vapors. Use protective goggles and gloves. Use in accordance with manufacturer's instructions.

- (3) Clean and dry area surrounding puncture using clean cloth soaked with solvent. Wipe off solvent. In shelters with RFI/EMI shielding, sand off all paint and foreign matter from face sheet surrounding damaged area at least 1-1/2 inches in all directions. Clean and dry bare metal.
- (4) Inject adhesive into puncture.
- (5) Apply a bead of adhesive approximately 1/4 inch wide over cuts in face sheet. Do not smooth out.

NOTE

In shelters having RFI/EMI shielding, perform steps (6) and (7) using electrically conductive tape, then repeat the procedure using non-conductive tape. In unshielded shelters, perform steps (6) and (7) only once using non-conductive tape.

- (6) Plan application of tape. Length and width, number of strips, overlaps and method of application will affect sealing capability of repair. Each piece of tape shall extend approximately 1-1/2 inches beyond adhesive. If width of damaged area exceeds width of tape, overlap tape strips at least 1/2 inch. If three or more strips of tape are required, apply center strip first.
- (7) Hold tape taut and apply lightly. Do not apply with rolling motion from end to end or side to side and do not rub strips into place. Rolling, rubbing and excessive pressure will squeeze adhesive out from under tape.
- (8) Touch up with paint as required (para 3-10).

3-10. Touchup Painting. When required to prevent rust and corrosion, touch up small areas of damaged or chipped paint in accordance with TM 43-0139. If a large area needs repainting, notify higher level of maintenance.

3-11. Door Brace Assembly.

This task covers: a. Service b. Remove c. Disassemble d. Assemble e. Install

INITIAL SETUP

<i>Tools</i>	<i>Materials/Parts</i>
General Mechanic's Automotive Tool Kit SC 5180-90-CL-N26	Sealer (Item 29 or 30, Appendix D) Cotter Pin MS24665-285 Lubricant (Item 17, Appendix D)

a. *Service.* Servicing of the door brace assembly consists of lubricating moving parts. Refer to paragraph 3-1 for lubrication instructions.

b. *Remove.* (figure 3-9)

- (1) Remove shoulder screw (1), self-locking nut (2) and flat washer (3) and detach upper brace (4) from door stop angle (5).
- (2) Remove wood screw (6) attaching chain end of chain and pin assembly (7) to door.


NOTE

If bracket (9) and screws (8) are in good condition and do not require replacement, omit step (3).

- (3) Remove ten screws (8) attaching bracket (9) to door and remove door brace assembly.

c. *Disassemble.* (figure 3-9)

- (1) Remove cotter pin (10) from pin of chain and pin assembly (7) and remove chain and pin assembly. Separate brace from bracket (9).
- (2) Push out roll pin(11) and remove catch (12).
- (3) Remove shoulder screw (13), self-locking nut (14) and flat washer (15) and separate upper brace (4) from lower brace (16).

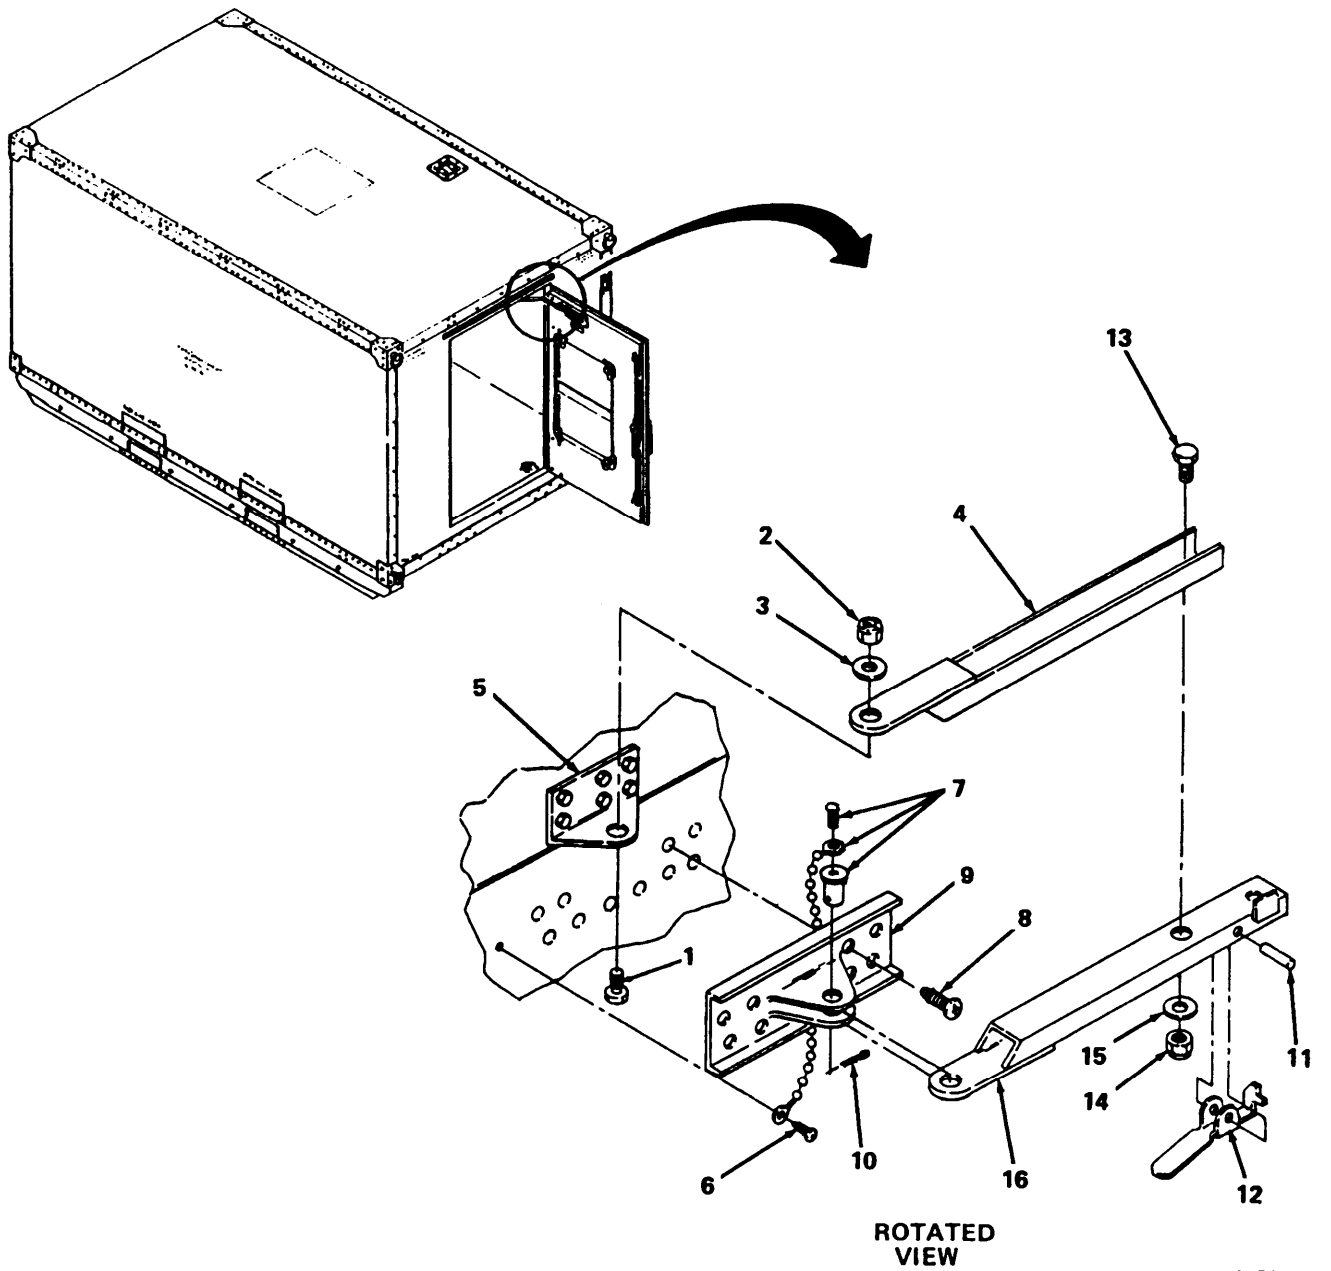

4753-013

Figure 3-9. Door Brace Assembly Removal and Disassembly.

3-11. Door Brace Assembly (cont).

d. Assemble. (figure 3-10)

- (1) Position upper brace (1) on lower brace (2) so that screw holes line up, and install shoulder screw (3), flat washer (4) and self-locking nut (5).
- (2) Position catch (6) on lower brace (2) and install roll pin (7).
- (3) Position tongue of lower brace (2) on bracket (8). Insert pin of chain and pin assembly (9) down through bracket and brace. Secure with cotter pin (10).

e. Install. (figure 3-10)

NOTE

If bracket (8) was not removed from door during removal, omit step (1).

- (1) Position bracket (8) on door and fasten with ten screws (11)
- (2) Mount chain end of chain and pin assembly (9) to door with wood screw (12).
- (3) Position free end of upper brace (1) against bottom of door stop angle (13) and install shoulder screw (14), flat washer (15) and self-locking nut (16).

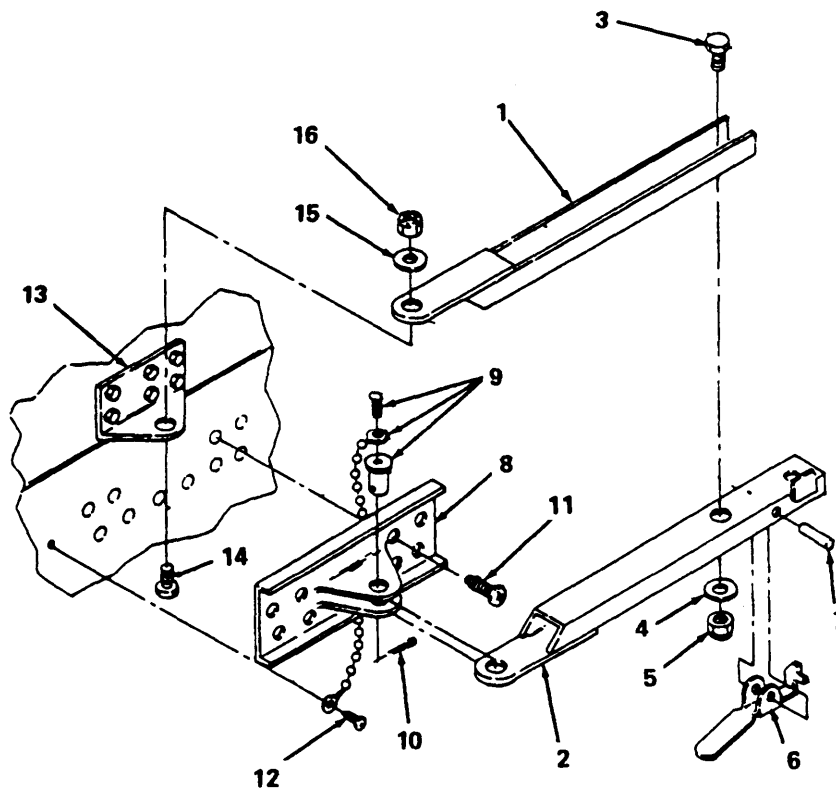


Figure 3-10. Door Brace Assembly Reassembly and Installation.

4753-014

3-12. Door Assembly.

This task covers: Service and Repair

INITIAL SETUP

Tools

Materials/Parts

As applicable

As applicable

Service and Repair. Service and repair of the door assembly is covered in the following referenced paragraphs:

- (1) Emergency exit panel assembly replacement (para 3-13).
- (2) T-latch and holder replacement para 3-14).
- (3) Door latch assembly repair and replacement (para 3-15).
- (4) Air inlet filter replacement (para 3-16).

3-13. Emergency Exit Panel Assembly.

This task covers: a. Service b. Repair c. Replace

INITIAL SETUP*Tools*

General Mechanic's Automotive Tool Kit
SC 5180-90-CL-N26

Materials/Parts

Lubricant (Item 17, Appendix D)

a. Service. Servicing of the emergency exit panel assembly consists of lubricating moving parts. Refer to paragraph 3-1 for lubrication instructions.

b. Repair. Repair of the emergency exit panel at unit level is limited to temporary repair of punctures in the aluminum. Refer to paragraph 3-9.c for repair procedures.

c. Replace. (figure 3-11)

- (1) Make sure emergency exit cover (1) is secured with latches (2) before removing emergency exit panel assembly (3) from door.
- (2) Remove four knobs (4) by turning each one Counterclockwise.
- (3) Pull emergency exit panel assembly (3) forward and out of door.
- (4) Position emergency exit panel assembly (3) in cutout in door.
- (5) install one knob (4) through each retainer (5) and into corner of emergency exit panel assembly (3) and tighten.

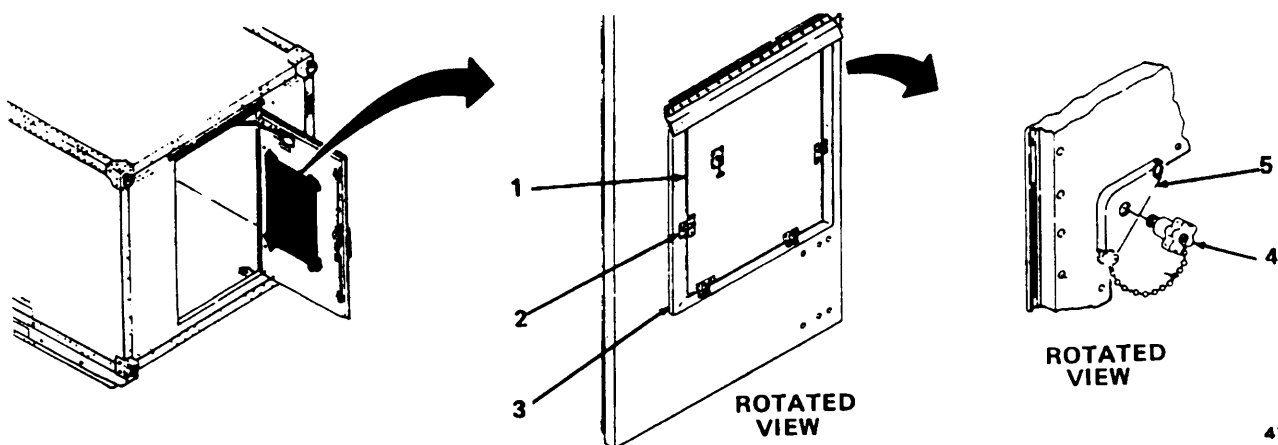


Figure 3-11. Emergency Exit Panel Assembly Replacement.

3-14. T-Latches and Holders.

This task covers: Replace

INITIAL SETUP

Tools

General Mechanic's Automotive Tool Kit
SC 5180-90-CL-N26

Materials/Parts

Sealer (Item 29 or 30, Appendix D)
Rivets, various
Goggles (Item 38, Appendix D)
Gloves (Item 12, Appendix D)

General Safety Instructions

WARNING

Drilling creates metal chips which may enter eyes and cause serious injury. Eye protection is required.

NOTE

The shelter has two T-latches. Replacement procedures are the same for both.

Replace. (figure 3-12)

- (1) Drill out four rivets (1) and remove T-latch (2). (Refer to paragraph 3-9a. for rivet removal instructions.)
- (2) Remove four screws (3), four flat washers (4), four lockwashers (5) and four nuts (6) and remove latch holder (7) from shelter wall.
- (3) Position latch holder (7) on shelter wall and fasten with four screws (3), four flat washers (4) four lockwashers (5) and four nuts (6).
- (4) Position T-latch (2) on shelter and fasten with four rivets (1). (Refer to paragraph 3-9a. for rivet installation instructions.)

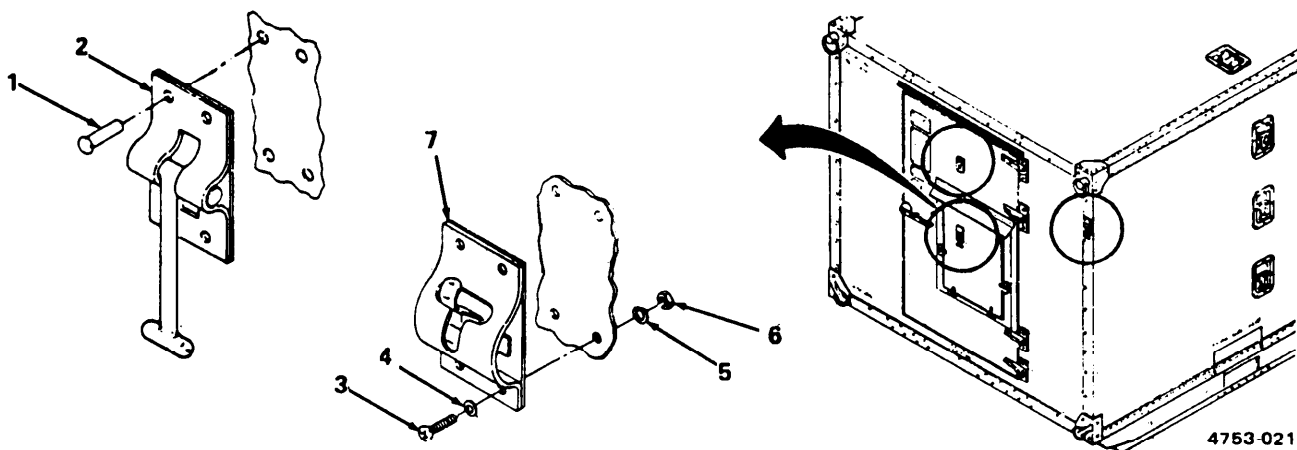


Figure 3-12. T-Latch and Holder Replacement.

3-15. Door Latch Assembly.

This task covers: a. Remove and Disassemble b. Inspect and Service c. Assemble and Install

INITIAL SETUP

<i>Tools</i>	<i>Materials/Parts</i>
General Mechanic's Automotive Tool Kit SC 5180-90-CL-N26	Keeper Shims, PN SC-B-200153 Lubricant, Silicone (Item 18, Appendix D) Sealer (Item 29 or 30, Appendix D) Shield Compound (Item 11, Appendix D) Washer Shims, PN SC-D-200140-8

a. Remove and Disassemble. (figure 3-13)

- (1) Push out three spring pins (1) and remove three pins (2) and three flat washers (3) attaching ends of latch rod assemblies (4) to latch arm assemblies (5). Remove latch rod assemblies.
- (2) Remove two self-locking nuts (6) and two flat washers (7) and remove upper and lower latch arm assemblies (5) from threaded ends of carriage bolts (8). Remove one spacer (9) from each latch arm assembly.

NOTE

Detent (10) is only located on bottom carriage bolt. Spacer(11) is only located on top carriage bolt.

- (3) Remove detent (10), spacer (11), shim washers (12) and spacers (13) from carriage bolts (8). Pull carriage bolts out of door.
- (4) Punch out spring pin (14) and take handle (15) off inside of door.
- (5) Punch out grooved pin (16) and take middle latch arm assembly (5) off inside of door.
- (6) Unscrew bearing sleeve nut (17) from handle shaft bearing sleeve (18) on inside of door.
- (7) Pull handle assembly (29 through 32) and handle shaft bearing sleeve (18) out of door.
- (8) Remove screw (19) and lockwasher (20), and remove padlock and key (21).
- (9) Remove two wood screws (22) and remove escutcheon plate (23) from outside of door.
- (10) Remove two cap screws (24) and two lockwashers (25) from each of three keepers (26) and remove keepers. Remove all shims (27). Record number and thickness of shims removed.
- (11) Remove latch lock assembly from middle (tapped) keeper (26) by unscrewing pin (28).

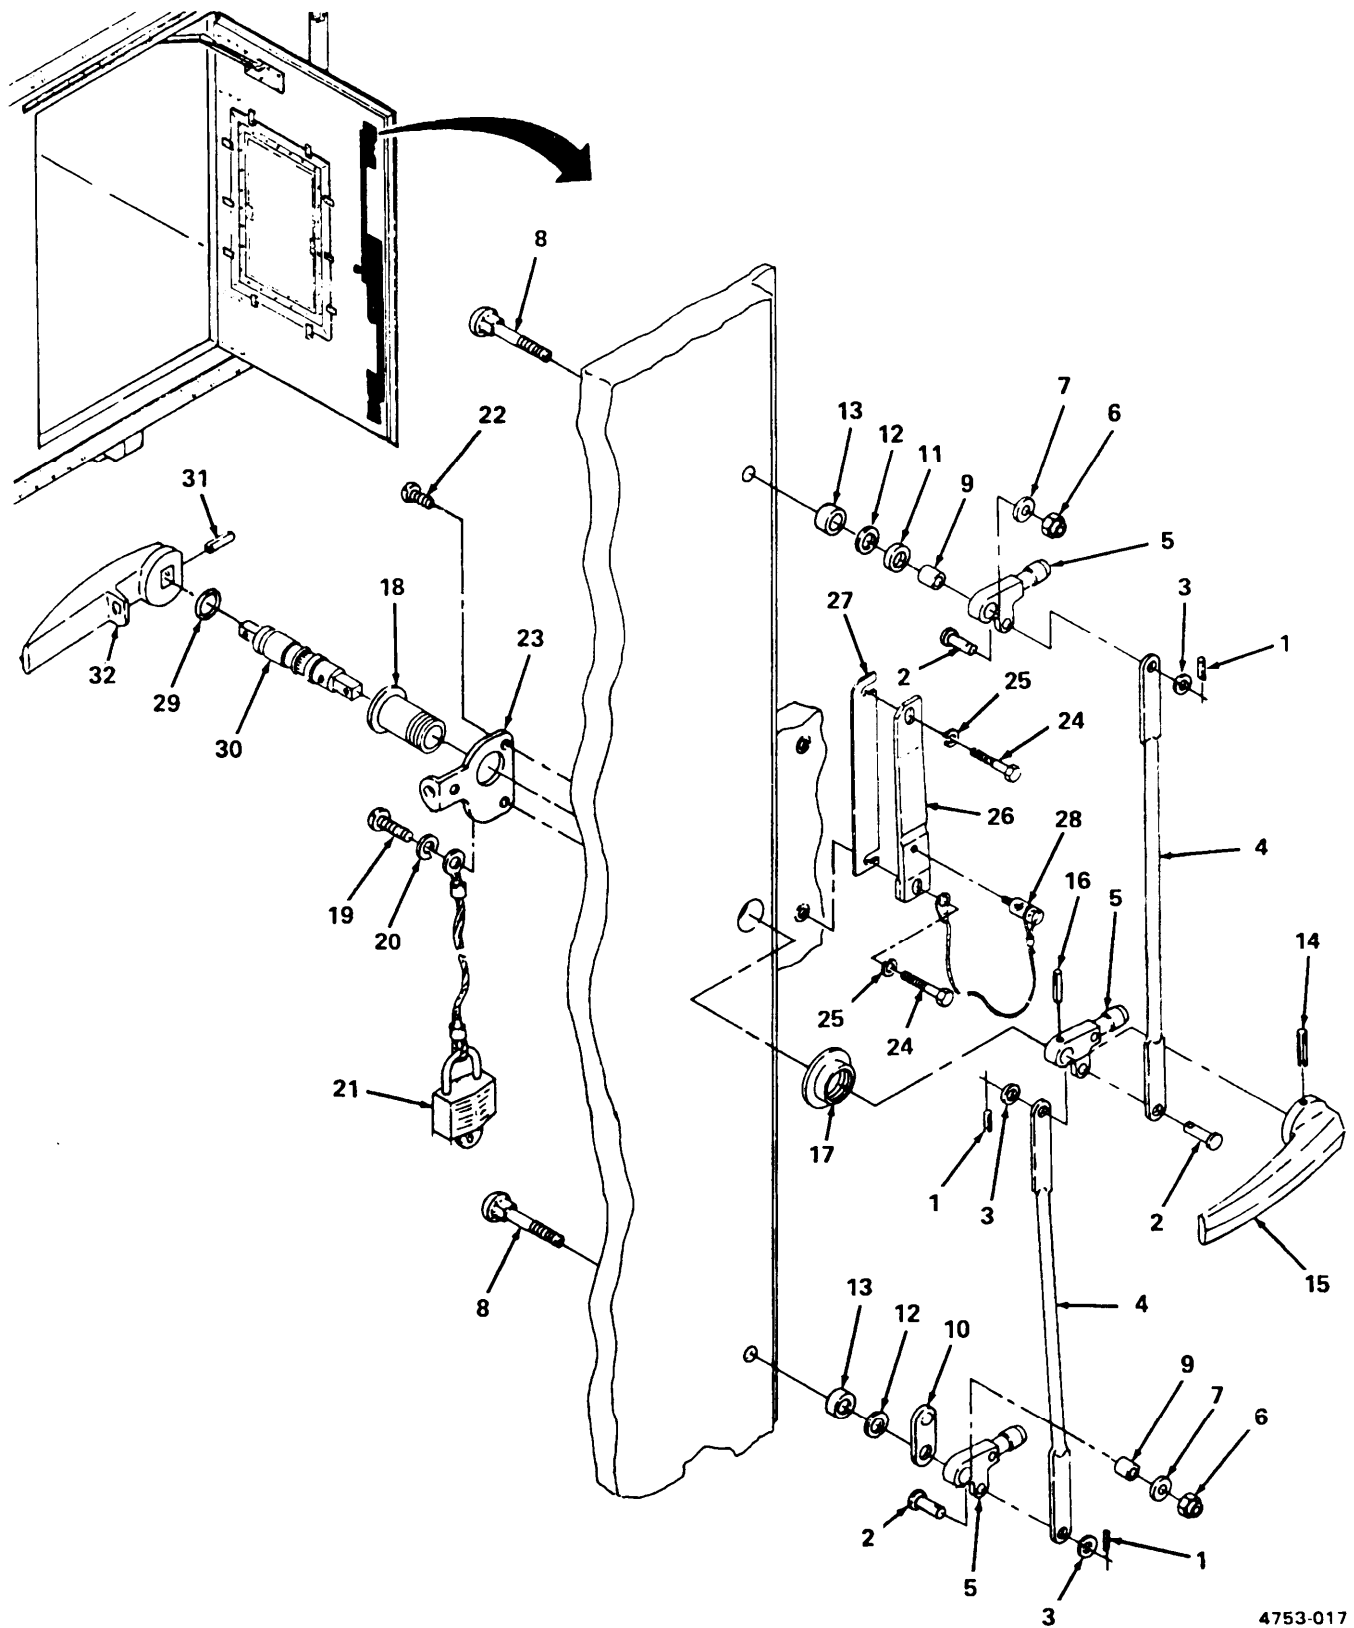


Figure 3-13. Door Latch Assembly Removal and Disassembly.

3-15. Door Latch Assembly (cont).

NOTE

Disassemble handle assembly (step (12)) only if damage is suspected.

- (12) Slip O-ring (29) off latch handle shaft (30). Punch out spring pin (31) and take handle (32) off latch handle shaft.

b. Inspect and Service.

- (1) Check condition of all pins. Replace any pin that is bent, corroded or otherwise deteriorated.
- (2) Clean and inspect threads of threaded parts. Inspect threaded inserts for thread damage and replace if necessary.
- (3) Lubricate all moving parts with silicone lubricant before reassembling.

c. Assemble and Install. (figure 3-14)

NOTE

If handle assembly (1) through (4)) was not disassembled during removal and disassembly, omit step (1).

- (1) Install handle (1) on latch handle shaft (2) so that pin holes line up. Insert spring pin (3). Slip O-ring (4) over latch handle shaft and into groove.

NOTE


Only the middle keeper is tapped for installation of a latch lock assembly.

- (2) Thread latch lock assembly pin (5) into tapped hole in tapped keeper (6).
- (3) Stack shim(s) (7) against bottom of keeper (6), using number and thickness of shims recorded during disassembly. Position tab (8) of latch lock assembly over mounting hole at raised end of keeper.

NOTE

Two different length screws are used to fasten the keeper.

- (4) Position keeper (6) and shims (7) on shelter wall so that mounting holes lineup and raised end of keeper is at the bottom. Install long screw (9) with lockwasher (10) through latch lock assembly tab (8) and raised end of keeper and into threaded insert in shelter wall. Install short screw (11) with lockwasher (10) in second mounting hole.
- (5) Repeat steps (3) and (4) for two remaining keepers (7), omitting latch lock assembly.

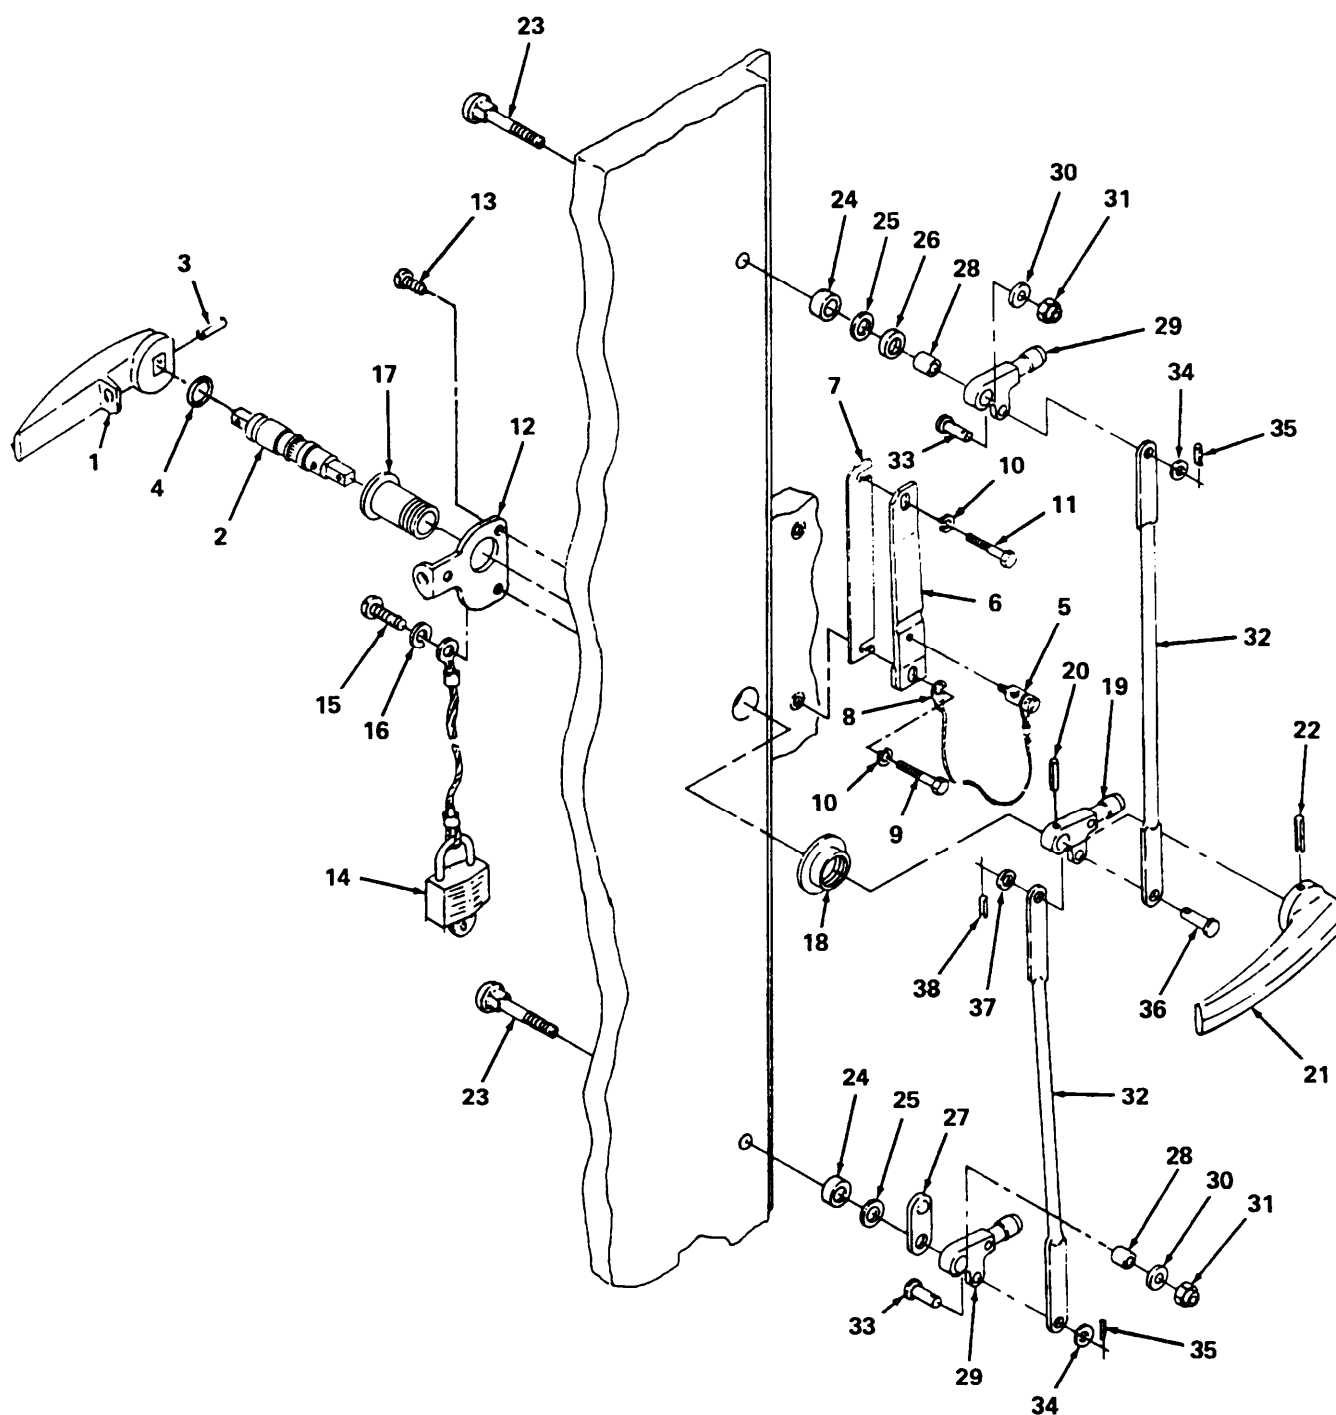

4753-018

Figure 3-14. Door Latch Assembly Reassembly and Installation.

3-15. Door Latch Assembly (cont).

NOTE

Use of shield compound is only required on RFI/EMI shielded shelters.

- (6) Apply shield compound to surface of door around handle mounting hole where surface will mate with escutcheon plate (12).
- (7) Position escutcheon plate (12) on outside of door over handle mounting hole and install two wood screws (13).
- (8) Position tab of padlock and key (14) over remaining mounting hole in escutcheon plate(12) and install screw (15) and lockwasher (16).
- (9) Apply shield compound to underside of flange of handle shaft bearing sleeve (17). Insert handle shaft bearing sleeve through door. Thread bearing sleeve nut (18) onto handle shaft bearing sleeve inside door and tighten until flange of handle shaft bearing sleeve tightens against escutcheon plate (12).
- (10) Insert handle assembly ((1) through (4)) into handle shaft bearing sleeve (17).
- (11) Position latch arm assembly (19) on handle assembly shaft (2) so that pin holes line up. Install grooved pin (20).
- (12) Position handle (21) on end of handle assembly shaft (2) so that pin holes line up. Install spring pin (22).

NOTE

Use same number of shim washers (25) with both carriage bolts (23).

- (13) Install two carriage bolts (23) in door. Install spacer (24) and shim washers (25) on each carriage bolt.
- (14) Install spacer (26) on top carriage bolt (23). Install detent (27) on bottom carriage bolt.
- (15) Insert one spacer (28) in each latch arm assembly (29). Position one latch arm assembly on each carriage bolt so that roller is pointing outboard. Secure each latch arm assembly with one flat washer (30) and one self-locking nut (31).
- (16) Measure distance between surface of each latch arm assembly (19 and 29) and plane of door surface. All three rollers should be aligned within .031 in (.079 cm). Add or subtract shims (25), as required, to achieve correct alignment.
- (17) Position one end of each latch rod assembly (32) against top and bottom latch arm assemblies (29) so that pin holes line up. Insert pins (33), install flat washers (34) and secure with spring pins (35).
- (18) Position remaining ends of each latch rod assembly (32) against middle latch arm assembly (19). Insert pin (36), install flat washer (37) and secure with spring pin (38).

- (19) Check latch torque. Latch torque should be 15 foot-pounds (max.) without RFI/EMI shielding gasket, or 30 foot-pounds (max.) with gasket installed. Adjust torque by adding or subtracting keeper shims (7).
- (20) Apply a bead of sealer around edges of escutcheon plate (12) and handle shaft bearing sleeve (17).
- (21) Lubricate as required (para 3-1).

3-16. Air Inlet Filters.

This task covers: a. Service b. Replace

INITIAL SETUP

Tools

General Mechanic's Automotive Tool Kit
SC 5180-90-CL-N26
Blind Riveter

Materials/Parts

Sealer (Item 29 or 30, Appendix D)
Rivnuts, various
Lubricant (Item 17, Appendix D)

Materials/Parts (cont)

Gloves (Item 12, Appendix D)
Goggles (Item 38, Appendix D)

General Safety Instructions

WARNING

Drilling creates metal chips which may enter eyes and cause serious injury. Eye protection is required.

a. Service. Servicing of the recessed step pan assembly consists of lubricating moving parts. Refer to paragraph 3-1 for lubrication instructions.

b. Replace (figure 3-15)

- (1) Drill out four rivets (1) and take divider strip (2) off frame (3). (Refer to paragraph 3-9a. for rivet removal instructions.)
- (2) Pull air filters (4) out of frame (3).
- (3) Insert air filters (4) into frame (3).
- (4) Position divider strip (2) across back against inside of frame flange, and fasten with four rivets(1). (Refer to paragraph 3-9a. for rivet installation instructions.)

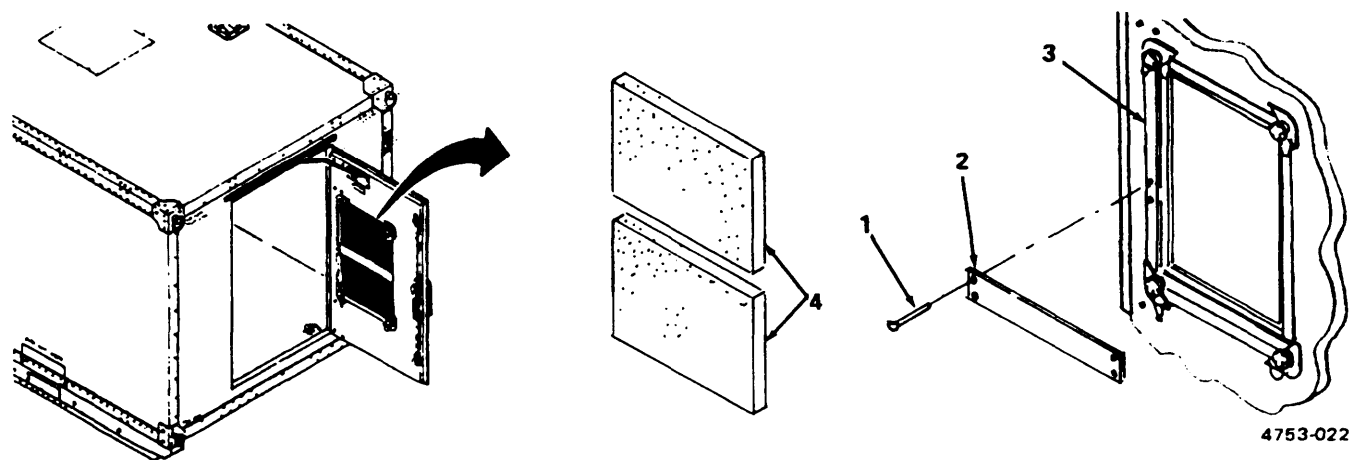


Figure 3-15. Air Inlet Filter Replacement.

3-17. Recessed Step Pan Assembly.

This task covers:

a. Service	b. Replace
------------	------------

INITIAL SETUP

Tools

General Mechanic's Automotive Tool Kit
SC 5180-90-CL-N26
Blind Riveter

Materials/Parts

Sealer (Item 29 or 30, Appendix D)
Rivnuts, various
Lubricant (Item 17, Appendix D)

Materials/Parts (cont)

Gloves (Item 12, Appendix D)
Goggles (Item 38, Appendix D)

General Safety Instructions

WARNING

Drilling creates metal chips which may enter eyes and cause serious injury. Eye protection is required.

NOTE

The shelter has three recessed step pan assemblies. This procedure is typical for all three.

a. *Service.* Servicing of the recessed step pan assembly consists of lubricating moving parts. Refer to paragraph 3-1 for lubrication instructions.

b. Replace. (figure 3-16)

- (1) Drill out ten rivets (1) and remove recessed step pan assembly (2) from shelter wall. (Refer to paragraph 3-9a for rivet removal instructions.)
- (2) Position recessed step pan assembly (2) in inset in shelter wall so that step is pointing up when retracted, and fasten with ten rivets (1). (Refer to paragraph 3-9a. for rivet installation instructions.)

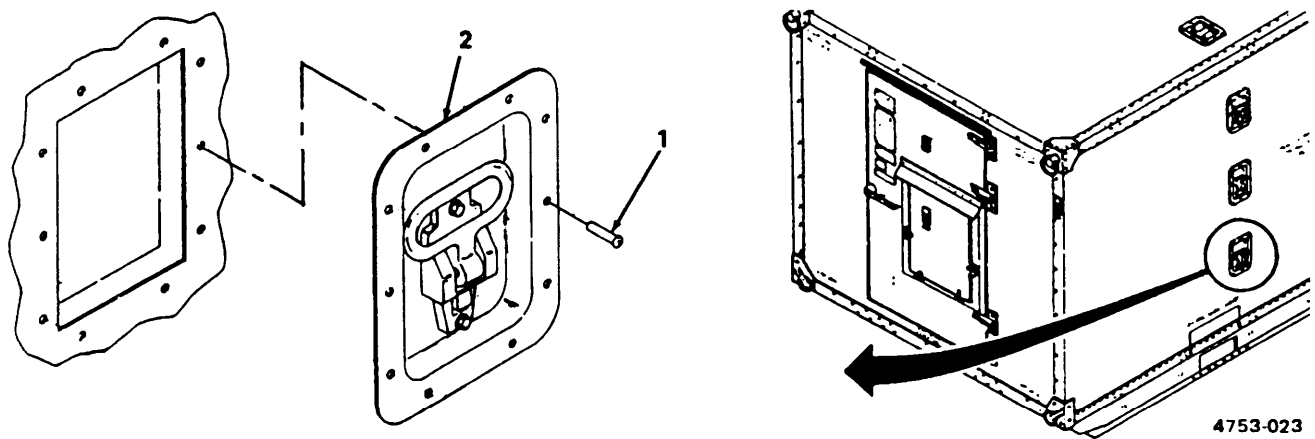


Figure 3-16. Recessed Step Pan Assembly Replacement.

3-18. D-Ring Assemblies (Hand Holds).

This task covers: a. Service b. Replace

INITIAL SETUP

Tools

General Mechanic's Automotive Tool Kit
SC 5180-90-CL-N26
Blind Riveter

Materials/Parts

Sealer (Item 29 or 30, Appendix D)
Rivnuts, various
Lubricant (Item 17, Appendix D)

Materials/Parts (cont)

Gloves (Item 12, Appendix D)
Goggles (Item 38, Appendix D)

General Safety Instructions

WARNING

Drilling creates metal chips which may enter eyes and cause serious injury. Eye protection is required.

NOTE

The shelter front wall has two D-ring assemblies and two D-rings with clamps. The shelter roof has one D-ring assembly that serves as a roof handle.

a. *Service.* Servicing of the hand holds consists of lubricating moving parts. Refer to paragraph 3-1 for lubrication instructions.


b. Replace. (figure 3-17)

- (1) Drill out four rivets (1) and remove D-ring assembly (2), or D-ring (3) and clamp (4), from shelter wall. (Refer to paragraph 3-9a. for rivet removal instructions.)
- (2) Drill out ten rivets (5) and remove hand hold D-ring assembly (6) from roof. (Refer to paragraph 3-9a. for rivet removal instructions.)

NOTE

The two rivets mounting the curbside edge of the hand hold (6) require a longer grip range than the remaining rivets.

- (3) Position hand hold D-ring assembly (6) in inset in roof and fasten with ten rivets (5). (Refer to paragraph 3-9a. for rivet installation instructions.)
- (4) Position D-ring (3) and clamp (4), or D-ring assembly (2), in inset in shelter and fasten with four rivets (1). (Refer to paragraph 3-9a. for rivet installation instructions.)
- (5) Lubricate as required (para 3-1).

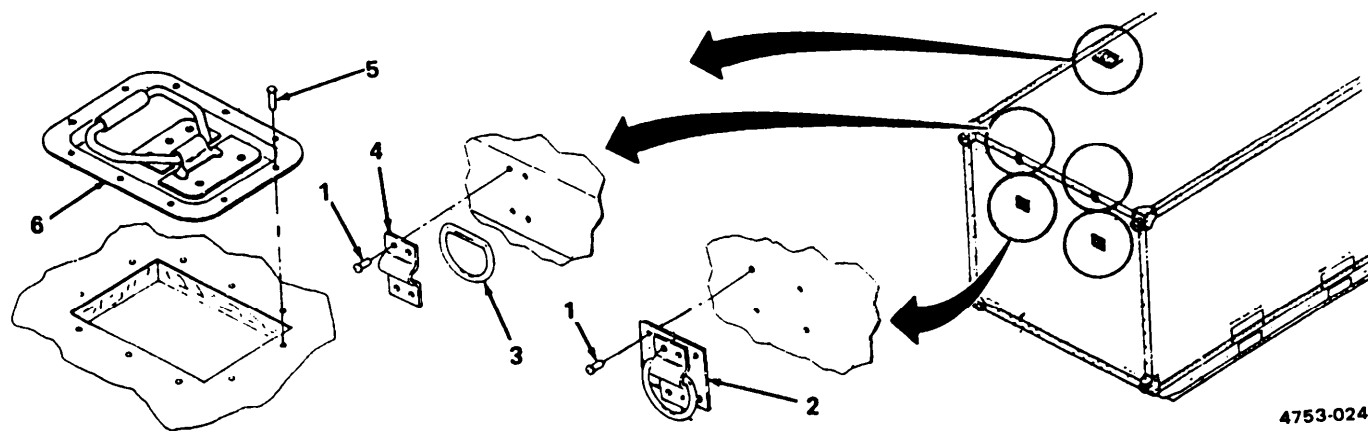

4753-024

Figure 3-17. D-Ring Assembly Replacement.

3-19. Drain Plug and EMI Washer.

This task covers: Replace

INITIAL SETUP

Tools

General Mechanic's Automotive Tool Kit
SC 5180-90-CL-N26

Materials/Parts

Sealer (Item 29 or 30, Appendix D)


Replace. (figure 3-18)

- (1) Unscrew wood screw (1) and pull drain plug (2) out of floor drain.

NOTE

Step (2) applies to S-280B/G Shielded shelters only.

- (2) Check condition of RFI/EMI washer (3) and replace if necessary.
- (3) Insert drain plug (2) firmly in floor drain.
- (4) Insert wood screw (1) through tab of drain plug chain and into floor.

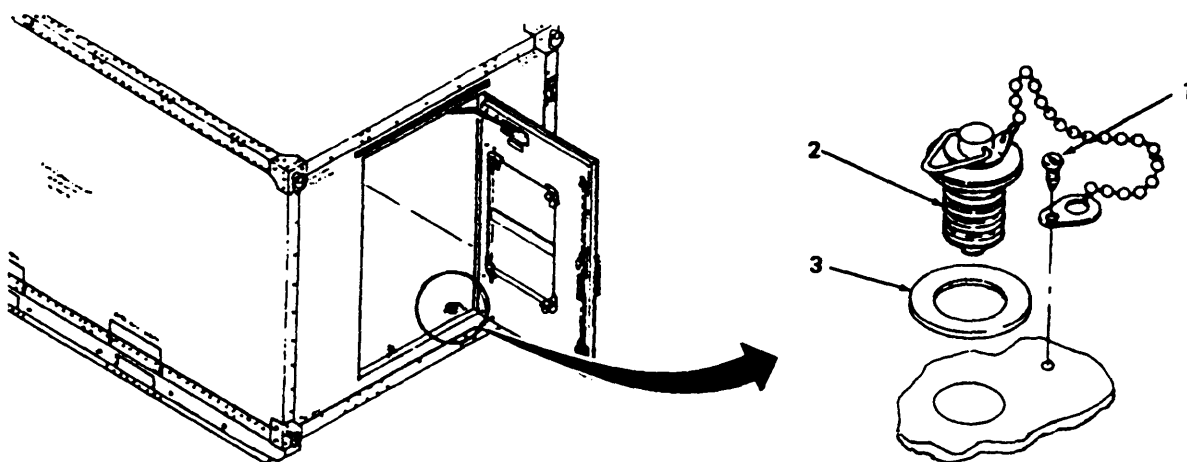

4753-025

Figure 3-18. Drain Plug and EMI Washer Replacement.

3-20. RFI/EMI Components.

This task covers: Replace

INITIAL SETUP*Materials/Parts*

Washer, PN SM-B-374181

Replace. RFI/EMI component replacement is limited to replacement of the EMI washer (para 3-19).

Section IV. PREPARATION FOR SHIPMENT AND STORAGE

Subject	Para	Page
General	3-21	3-35
Loading Shelter into ANSI/ISO Container	3-22	3-35
General Storage Requirements	3-23	3-35
Administrative Storage	3-24	3-35

3-21. General. No special preparation is required for shipment of the shelter other than making sure the correct sling assembly is available and in good condition, the skids are in good condition and securely mounted to the shelter, and the drain plug is loosened for air or rail transport.

3-22. Loading Shelter into ANSI/ISO Container. Shelters maybe shipped in Type IAA ANSI/ISO containers only when crated or pallet-mounted. Block crates or pallets securely in the container to prevent movement and damage during transit. Install and remove shelters in accordance with TB 11-5400-200-14.

3-23. General Storage Requirements. Accumulation of moisture within the shelter resulting from temperature and humidity fluctuations can damage equipment. Minimize moisture accumulation by keeping shelter doors, louver covers and drain holes open during indoor storage. During outdoor storage, keep doors and drain holes closed, but keep louver covers open. A free breather assembly may also be used, when available, to absorb moisture inside the shelter. When using the free breather assembly, doors, louver covers and drain holes must be closed. For usage information, refer to the applicable drawing for the particular free breather assembly being used.

3-24. Administrative Storage.

a. Placement of equipment in administrative storage should be for short periods of time when a shortage of maintenance effort exists. Items should be in mission readiness within 24 hours or within the time factors as determined by the directing authority. During the storage period appropriate maintenance records will be kept.

b. Before placing equipment in administrative storage, current maintenance services and equipment serviceable criteria (ESC) evaluations should be completed, shortcomings and deficiencies should be corrected, and all modification work orders (MWO's) should be applied.

c. Storage site selection. Inside storage is preferred for items selected for administrative storage.

CHAPTER 4

DIRECT SUPPORT MAINTENANCE INSTRUCTIONS

Subject	Section	Page
Repair Parts, Special Tools, TMDE and Support Equipment.	I	4-1
Troubleshooting	II	4-1
Direct Support Maintenance procedures.	III	4-3

Section I. REPAIR PARTS, SPECIAL TOOLS, TMDE AND SUPPORT EQUIPMENT

Subject	Para	Page
Common Tools.	4-1	4-1
Special Tools, TMDE and Support Equipment.	4-2	4-1
Repair Parts.	4-3	4-1

4-1. **Common Tools.** A complete list of common tools and tool kits is given in Section III of Appendix B, Maintenance Allocation.

4-2. **Special Tools,** TMDE and Support Equipment. There are no special tools or equipment needed to maintain the shelters.

4-3. **Repair Parts.** Repair parts for direct support maintenance of the shelters are listed and illustrated in TM 10-5411-206-24P.

Section II. TROUBLESHOOTING

4-4. **Troubleshooting.** This section contains troubleshooting information for malfunctions which may develop in the shelters. Fault isolation is limited to those components which may be repaired or replaced at the direct support level. Table 4-1 lists the common malfunctions you may encounter during operation or maintenance of the shelter. Each malfunction is followed by a list of tests or inspections and corrective actions. These tests or inspections and corrective actions should be performed in the order listed. This manual cannot list all malfunctions that may occur. If you encounter a malfunction that is not listed or cannot be corrected by the listed corrective actions, notify your supervisor.

Table 4-1. Troubleshooting.

MALFUNCTION	TEST OR INSPECTION	CORRECTIVE ACTION
1. WATER IS GETTING INTO SHELTER		
	Step 1. Check condition of weather gaskets on door and emergency exit panel.	Replace deteriorated gaskets (para 4-12).
	Step 2. Check condition of drip cap and drip mold.	Replace defective drip cap (para 4-13) or drip mold (para 4-7).
	Step 3. Inspect shelter walls and ceiling for leaks.	Patch any holes (para 4-20).
	Step 4. Check to see that all exterior wall and ceiling patches are firmly mounted and bonded to shelter wall.	Apply sealer around edge of patch, or replace patch (para 4-20).
	Step 5. Check to see if louver assembly is installed backwards. Louvers should aim down toward the outside.	Remove intake louver assembly and reinstall correctly (para 4-15).
	Step 6. Check to see if lifting eye assemblies or towing eye assemblies have pulled away from shelter corners.	<ul style="list-style-type: none"> a. Apply sealer to gaps around bracket edges. b. If replacement is required, notify higher level of maintenance.
2. THERE IS EVIDENCE OF RADIO FREQUENCY/ELECTROMAGNETIC INTERFERENCE (S-280B/G SHIELDED)		
	Step 1. Inspect shelter walls, ceiling and floor for holes.	Patch any holes (para 4-20).
	Step 2. Check to see that all exterior wall and ceiling patches are firmly mounted and bonded.	Replace poorly mounted patches and replace all temporary tape patches with permanent aluminum patches (para 4-20).

Table 4-1. Troubleshooting (cont).

MALFUNCTION	TEST OR INSPECTION	CORRECTIVE ACTION
	Step 3. Check condition of RFI/EMI filter in door.	Replace damaged or missing filter (para 4-15).
	Step 4. Check for missing hinge shims.	Replace missing shims (para 4-17).
	Step 5. Check condition of metal door gasket.	If replacement is required, notify higher level of maintenance.

Section III. DIRECT SUPPORT MAINTENANCE PROCEDURES

Subject	Para	Page
General	4-5	4-3
Surface Preparation, Priming and Painting	4-6	4-3
Drip Mold	4-7	4-4
Data Plates	4-8	4-5
Door Stop Angle	4-9	4-6
Floor Tread	4-10	4-7
Door Assembly	4-11	4-8
Weather Gaskets	4-12	4-9
Drip Cap	4-13	4-11
Emergency Exit Latches, Strikes and Stud Plate Assemblies	4-14	4-12
Intake Louver Assembly and RFI Fitter	4-15	4-14
Door Knob Assemblies	4-16	4-16
Door Hinge Assemblies	4-17	4-18
Door Skin	4-18	4-20
RFI/EMI Components	4-19	4-21
Wall Floor and Ceiling Panels	4-20	4-22

4-5. **General** This section contains maintenance procedures which are the responsibility of direct support maintenance, as authorized by the Maintenance Allocation Chart (appendix B). The general maintenance information given for unit level maintenance also applies to direct support level maintenance. This information is contained in paragraph 3-8.

4-6. **Surface Preparation, Priming and Painting.** All bare metal shall be painted to prevent corrosion. Touch up small dents and chips. Repaired sections of panels must be prepared with a corrosion protection primer before painting. Do not attempt to repaint large areas such as complete exterior, interior ceiling. Detailed priming and painting instructions can be found in TM43-0139.

4-7. Drip Mold.

This task covers: Replace

INITIAL SETUP

Tools

Electronic Equipment Shelter Tool Kit TK-1 44/G
General Mechanic's Automotive Tool Kit
SC 5180-90-CL-N26
Blind Riveter

General Safety Instructions

WARNING

Drilling creates metal chips which may enter eyes and cause serious injury. Eye protection is required.

Materials/Parts

Sealer (Item 29 or 30, Appendix D)
Rivets, Various
Goggles (Item 38, Appendix D)


Replace. (figure 4-1)

- (1) Drill out seven rivets (1 and 2) and remove drip mold (3) from shelter wall. (Refer to paragraph 3-9.a for rivet removal instructions.)

NOTE

The last two rivet locations on each end of drip mold require longer grip range rivets than the middle three locations.

- (2) Position drip mold (3) on shelter wall and fasten with four long rivets (1) and three short rivets (2). (Refer to paragraph 3-9.a for rivet installation instructions.)

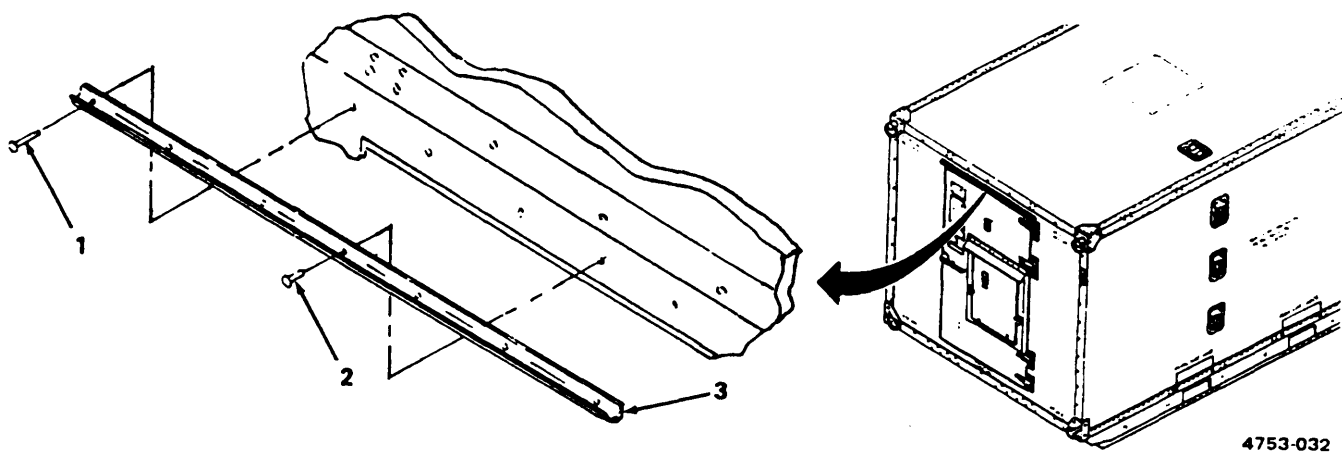

4753-032

Figure 4-1. Drip Mold Replacement.

4-8. Data Plates.

This task covers: Replace

INITIAL SETUP

Tools

Electronic Equipment Shelter Tool Kit
TK-144/G
General Mechanic's Automotive Tool Kit
SC 5180-90-CL-N26
Blind Riveter

General Safety Instructions

WARNING

Drilling creates metal chips which may enter eyes and cause serious injury. Eye protection is required.

Materials/Parts

Sealer (Item 29 or 30, Appendix D)
Rivets, Various
Goggles (Item 38, Appendix D)

Replace. (figure 4-2)

- (1) Drill out four rivets (1) and remove plate (2, 3, 4, 5 or 6) from shelter wall. (Refer to paragraph 3-9.a for rivet removal instructions.)
- (2) Position data plate (2, 3, 4, 5 or 6) on shelter wall and fasten with four rivets (1). (Refer to paragraph 3-9.a for rivet installation instructions.)

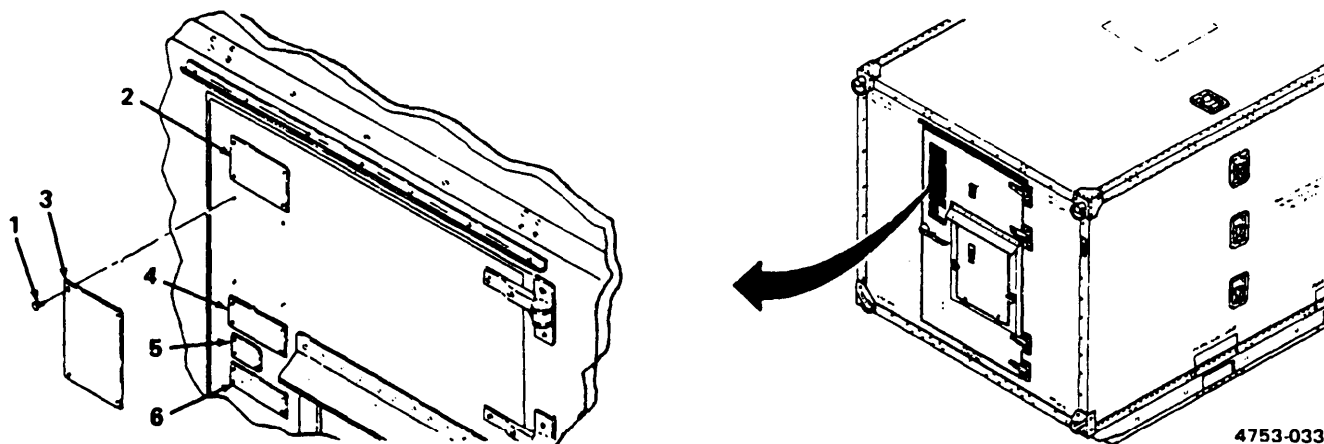


Figure 4-2. Data Plate Replacement.

4-9. Door Stop Angle.

This task covers: Replace

INITIAL SETUP

Tools

Electronic Equipment Shelter Tool Kit
TK-144/G
General Mechanic's Automotive Tool Kit
SC 5180-90-CL-N26
Blind Riveter

Materials/Parts

Sealer (Item 29 or 30, Appendix D)

Replace. (figure 4-3)

- (1) Remove shoulder screw (1), self-locking nut (2) and flat washer (3) and swing door brace (4) away from door stop angle (5).
- (2) Remove six bolts (6) and take door stop angle (5) off shelter wall.
- (3) Inspect rivnuts (7) and replace if necessary (para 3-9. b).
- (4) Position door stop angle (5) on shelter wall so that mounting holes line up with rivnuts (7) over door.
- (5) Install six bolts (6).
- (6) Position door brace (4) against underside of door stop angle (5) and fasten with shoulder screw (1), flat washer (3) and self-locking nut (2).

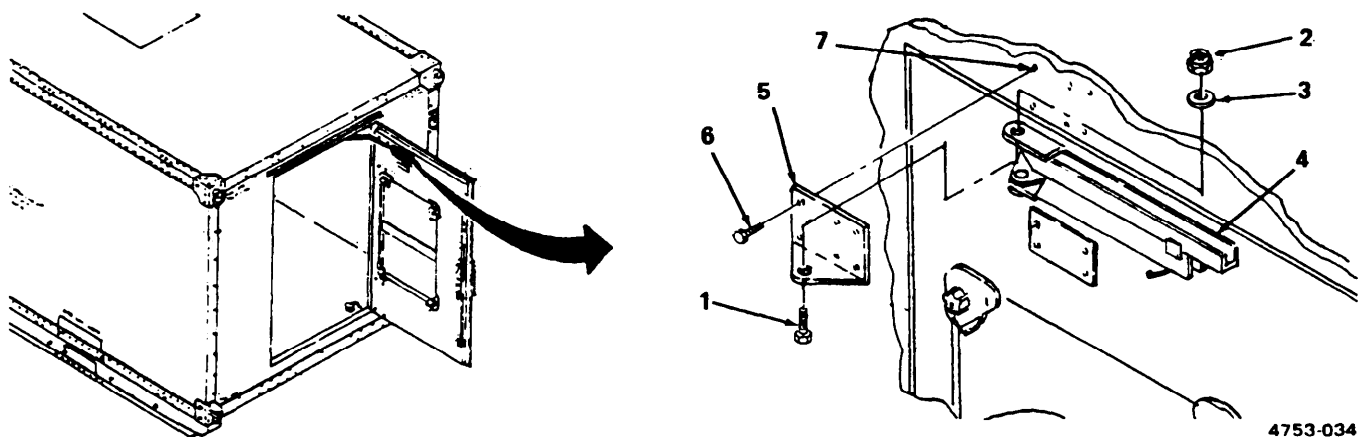


Figure 4-3. Door Stop Angle Replacement.

4-10. Floor Tread.

This task covers: Replace

INITIAL SETUP*Tools*

Electronic Equipment Shelter Tool Kit
TK-144/G
General Mechanic's Automotive Tool Kit
SC 5180 -90-CL-N26

Materials/pads

Solvent (Item 37, Appendix D)
Rubber Floor Matting (Item 19 or 20, Appendix D)
Gloves (Item 12, Appendix D)
Goggles (Item 38, Appendix D)

*General Safety /nstructions***WARNING**

Solvents are flammable. Keep away from heat and open flames. Avoid eye and skin contact and breathing of vapors. Use protective goggles and gloves. Use in a well-ventilated area. Use in accordance with manufacturer's instructions.

*Replace.***CAUTION**

When removing floor tread that has been cemented down, be careful not to delaminate shelter floor.

NOTE

When installing new floor tread inside shelter, it is not necessary to remove old, worn floor tread that has been cemented down unless leaving it in place and covering it with new tread material will interfere with equipment or racks. If old tread is not being removed, omit steps (1) through (3).

- (1) Remove old floor tread completely.

CAUTION

Do not permit solvent to penetrate through floor panels. Solvent may dissolve core material.

- (2) Remove residue using solvent. Wipe off solvent.

- (3) Prime and paint floor (para 4-6).

- (4) Cut new floor tread using 1/8 or 3/16 inch thick rubber floor matting. Lay new tread in place. Do not cement in place.

4-11. Door Assembly.

This task covers: Repair

INITIAL SETUP

Tools

As required

General Safety Instructions

WARNING

Materials/Parts

As required

Adhesives contain toxic solvents. Avoid eye and skin contact and breathing of vapors. Use in a well-ventilated area. Use protective goggles and gloves. Use in accordance with manufacturer's instructions.

Drilling creates metal chips which may enter eyes and cause serious injury. Eye protection is required.

Repair. Repair of the door assembly is covered in the following referenced paragraphs:

- (1) Weather gasket replacement (para 4-12).
- (2) Drip cap replacement (para 4-13).
- (3) Emergency exit latch, strike and stud plate assembly replacement (para 4-14).
- (4) Intake louver assembly and RFI filter replacement (para 4-15).
- (5) Doorknob assembly replacement (para 4-16).
- (6) Door hinge assembly replacement (para 4-17).
- (7) Door Skin (para 4-18).

4-12. Weather Gaskets.

This task covers: Replace

INITIAL SETUP

Tools

General Mechanic's Automotive Tool Kit
 SC 5180-90-CL-N26
 Electronic Equipment Shelter Tool Kit TK-144/G

Materials/Parts

Gasket, (Item 13, Appendix D)
 Solvent (Item 37, Appendix D)
 Adhesive (Item 2,3,4 or 5, Appendix D)
 Primer (Item 23, Appendix D)
 Gloves (Item 12, Appendix D)
 Goggles (Item 38, Appendix D)

General Safety Instructions

WARNING

Solvents and adhesives are flammable and toxic. Keep away from heat and open flames. Avoid eye and skin contact and breathing of vapors. Use in a well-ventilated area. Use protective goggles and gloves. Use in accordance with manufacturer's instructions.

Replace (figure 4-4)

NOTE

Gaskets must be replaced when a permanent set occurs and the seal is no longer reliable. Weather gaskets can be found on the door assembly and emergency exit (inlet assembly). Replacement procedures are the same for all weather gaskets.

- (1) Carefully remove gasket and scrape channel clean.
- (2) Remove residue using solvent.

NOTE

Adhesive must be applied between 30 minutes and eight hours after application of primer. If original primer coat was not damaged during removal of old gasket, it is not necessary to apply new coat of primer.

- (3) Apply primer, then adhesive, evenly to sides and bottom of gasket channel to insure a continuous bond.
- (4) Immediately after applying adhesive, press new gasket into place.
- (5) Clamp gasket around each corner to ensure good gasket contact with channel bottom while adhesive cures. Gasket surface which mates with door jamb must be flat with no sharp discontinuities along its length, corners or joint while adhesive cures.

4-12. Weather Gaskets (cont).

- (6) Allow adhesive to cure at least 12 hours at 50% RH and 70°F (21°C). Lower humidity and temperatures require a longer cure time.
- (7) After adhesive has cured, fill gasket channel voids at each corner with adhesive so that it is flush with door. Bond gasket ends together with adhesive to form a tight joint. Do not fill gasket hollow section at joint.
- (8) Test gasket seating by inserting a piece of paper 0.005 inch (maximum) thick by 2-1/2 inches wide at center of top and bottom of door or cover and three places along each side. When door or cover is closed, paper should be trapped between weather gasket and mating surface (but not under RFI/EMI gasket in shielded shelters). If paper can be withdrawn without any resistance while door or cover is closed, gasket is not making good contact with mating surface. Correct as follows:
 - (a) Check condition of gasket. Replace gasket if it is in unsatisfactory condition, or if it is improperly installed (kinked or poorly spliced).
 - (b) If gasket is in good condition, gasket compression maybe increased by changing thickness of latch keeper shims (para 3-15) or hinge shims (para 4-17). Make sure latches contact their respective keepers when closed.
 - (c) After adjustments are made, make sure door cover is capable of opening and closing fully without binding.
 - (d) Repeat gasket seating test.

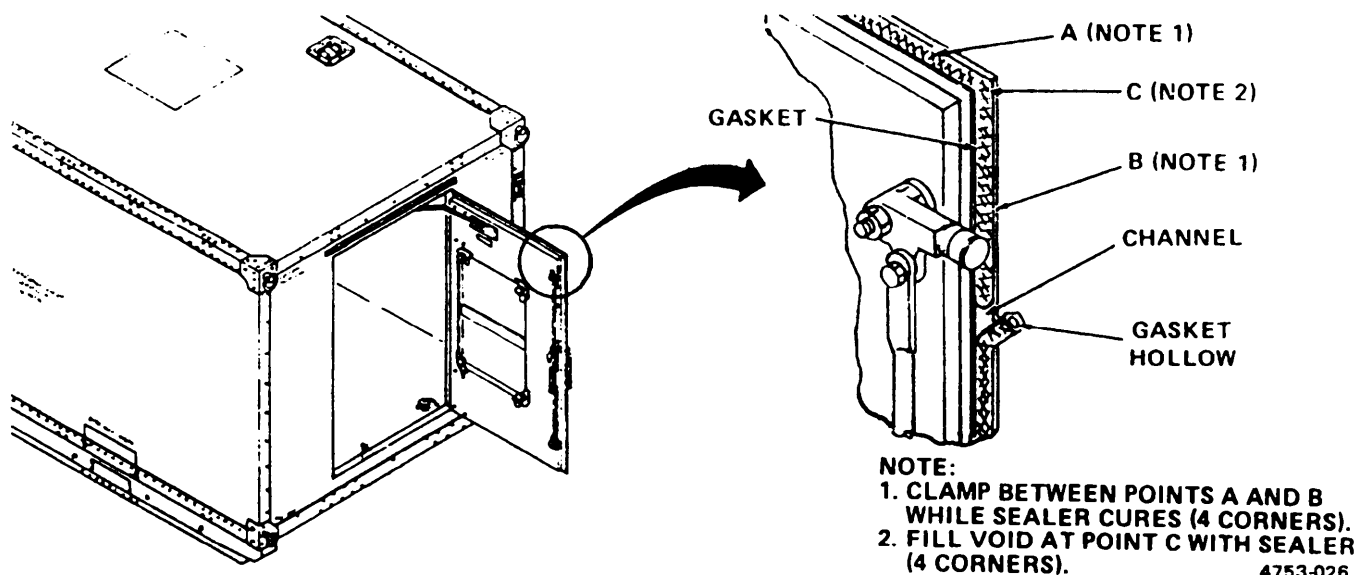


Figure 4-4. Weather Gasket Replacement.

4-13. Drip Cap.

This task covers: Replace

INITIAL SETUP

Tools

General Mechanic's Automotive Tool Kit
 SC 5180 -90-CL-N26
 Electronic Equipment Shelter Tool Kit TK-144/G
 Blind Riveter

Materials/Parts (cont)

Rubber, Synthetic (Item 38, Appendix D)
 Goggles (Item 38, Appendix D)
 General Safety Instructions

Materials/Parts

Sealer (Item 29 or 30, Appendix D)
 Rivnuts, various

WARNING

Drilling creates metal chips which may enter eyes and cause serious injury. Eye protection is required.

Replace (figure 4-5)

- (1) Drill out 17 rivets (1) and take drip cap strip (2) and drip cap (3) off door. (Refer to paragraph 3-9.a. for rivet removal instructions.)
- (2) Cut a new drip cap (3) out of rubber, using old drip cap as a template.
- (3) Using drip cap strip (2) as a template, punch 17 holes in edge of replacement drip cap (3).
- (4) Position drip cap (3) and strip (2) on shelter door and fasten with 17 rivets (1). (Refer to paragraph 3-9.a. for rivet installation instructions.)

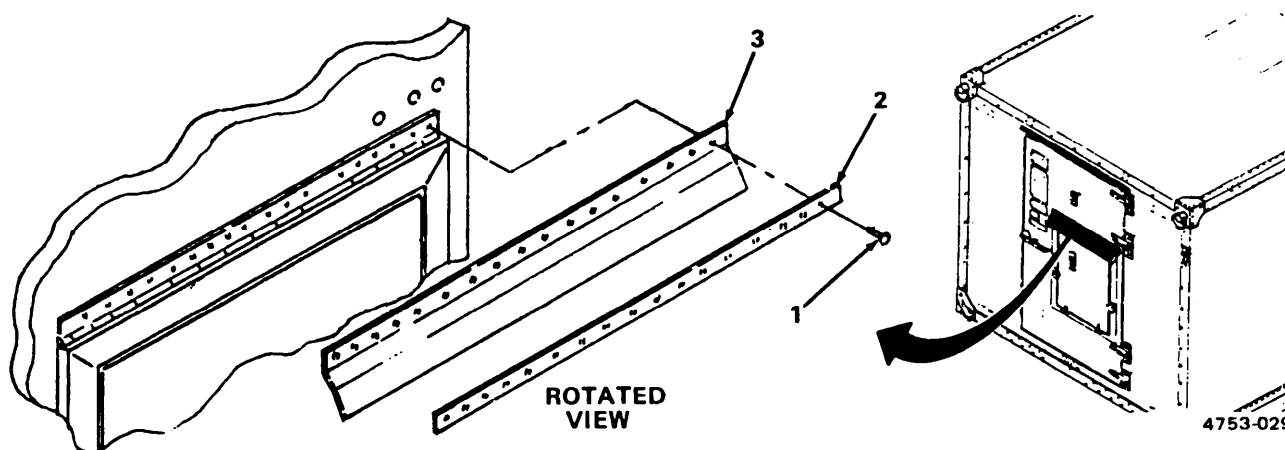


Figure 4-5. Drip Cap Replacement.

4-14. Emergency Exit Latches, Strikes and Stud Plate Assemblies

This task covers: Replace

INITIAL SETUP

Tools

General Mechanic's Automotive Tool Kit
SC 5180 -90-CL-N26
Blind Riveter

Materials/Parts

Sealer (Item 29 or 30, Appendix D)
Rivnuts, various
Goggles (Item 38, Appendix D)

General Safety Instructions

WARNING

Drilling creates metal chips which may enter eyes and cause serious injury. Eye protection is required.

Replace (figure 4-6)

NOTE

There are four latches, strikes and stud plate assemblies on the emergency exit panel.
This procedures is typical for all four.

- (1) Remove self-locking nut (1) and flat washer (2) and take latch (3) and flat washer (4) off stud plate assembly (5).
- (2) Drill out two rivets (6) and remove stud plate assembly (5) from frame (7) of emergency exit panel. (Refer to paragraph 3-9.9 for rivet removal instructions.)
- (3) Drill out three rivets (8 and 9) and remove strike (10) from emergency exit panel cover (1 1). (Refer to paragraph 3-9a. for rivet removal instructions.)
- (4) Position strike (1 O) on emergency exit panel cover (1 1) and fasten with two countersunk head rivets (8) and one dome head rivet (9). (Refer to paragraph 3-9a. for rivet installation instructions.)
- (5) Position stud plate assembly (5) on frame (7) of emergency exit panel and fasten with two rivets (6). (Refer to paragraphs 3-9a. for rivet installation instructions.)
- (6) Slide flat washer (4), then latch (3), then second flat washer (2) onto stud of stud plate assembly (5). Secure with self-locking nut (1). Make nut just loose enough to permit hand operation of latch.

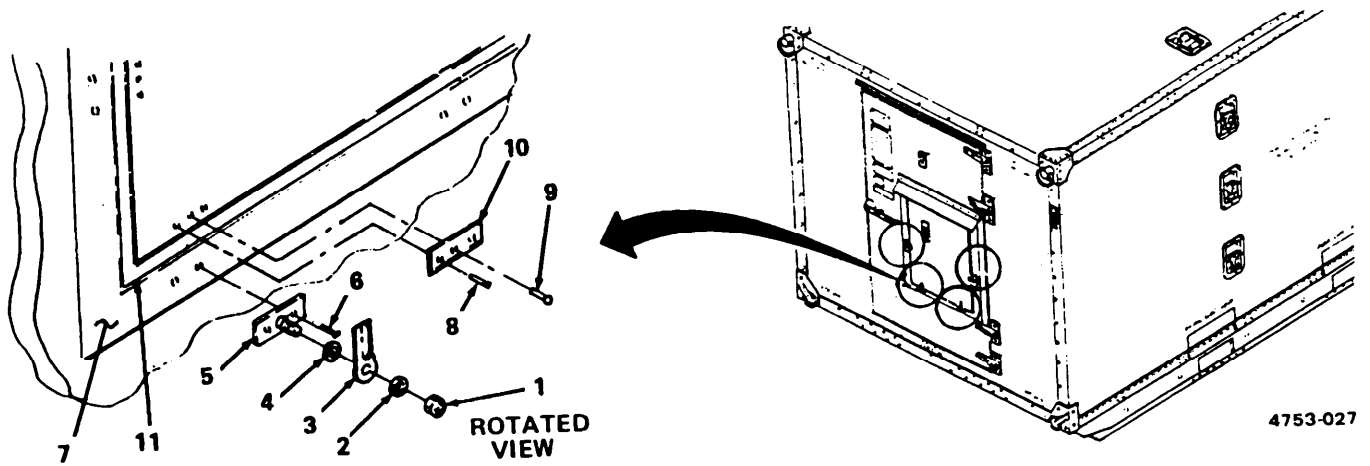


Figure 4-6. Emergency Exit Latch Strike and Stud Plate Assembly Replacement

4-15. Intake Louver Assembly and RFI/EMI Filter.

This task covers: Replace

INITIAL SETUP

<i>Tools</i>	<i>Personnel Required</i>
General Mechanic's Automotive Tool Kit SC 5180-90-CL-N26	Two
Electronic Equipment Shelter Tool Kit TK-144/G	Equipment Condition
<i>Materials/Parts</i>	
Sealer (Item 29 or 30, Appendix D) Tape SM-B-450436-1	Air inlet filter removed (para 3-16)

Replace (figure 4-7)

NOTE

Shielded shelters have an RFI/EMI filter mounted to the emergency exit frame, between the intake louver and the air inlet filter. When replacing the intake louver in a shelter without RFI/EMI shielding, omit the steps in this procedure that pertain to the RFI/EMI fitter and tape.

- (1) Prop emergency exit cover (1) open.
- (2) Working on inside of emergency exit, unscrew 92 slotted screws (2), while assistant supports intake louver assembly (3) from outside.
- (3) Working on outside of emergency exit, take four retaining strips (4 and 5), intake louver assembly (3) and RFI/EMI filter (6) off frame (7). Peel off tape.
- (4) Install tape on all mating surfaces between frame (7) and flange of RFI/EMI filter (6).

NOTE


Make sure sealer is still wet when installing intake louver assembly (3) and retaining strips (4 and 5).

- (5) Coat both sides of flange of intake louver assembly (3) with sealer.
- (6) Working on outside of emergency exit, position RFI/EMI filter (6) against back of intake louver assembly (3) so that mounting holes in flanges line up.
- (7) While assistant holds intake louver assembly (3) and RFI/EMI filter (6) in position against frame (7), install eight comer slotted screws (2) from interior side of emergency exit.

- (8) Position retaining strips (4 and 5) on flange of intake louver assembly (3) so that previously installed corner screws (2) pass through end mounting holes of each retaining strip.
- (9) Working on inside of emergency exit, install remaining slotted screws (2).
- (10) Apply a bead of sealer around edge of flanges of intake louver assembly (3) and RFI/EMI filter (6).
- (11) Close emergency exit cover (1).

NOTE

FOLLOW-ON MAINTENANCE: Install air inlet filter (para 3-16).

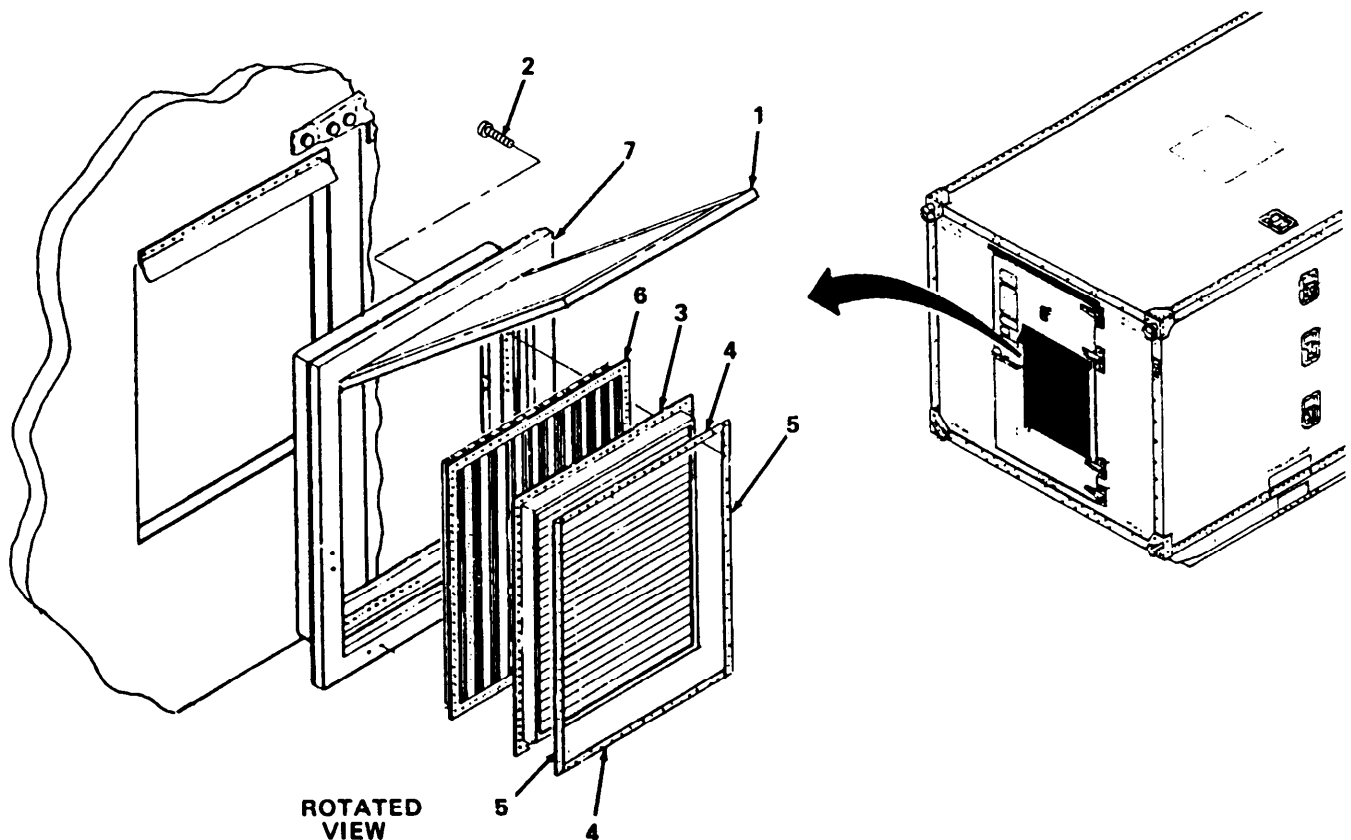

4753-028

Figure 4-7. Intake Louver Assembly and RFI/EMI Filter Replacement.

4-I6. Door Knob Assemblies.

This task covers: Replace

INITIAL SETUP

Tools

General Mechanic's Automotive Tool Kit
SC 5180 -90-CL-N26
Blind Riveter

Materials/Parts

Sealer (Item 29 or 30, Appendix D)
Rivnuts, various
Goggles (Item 38, Appendix D)

General Safety Instructions

WARNING

Drilling creates metal chips which may enter eyes and cause serious injury. Eye protection is required.

NOTE

There are four knob assemblies on inside of shelter door. This procedure is typical for all four.

Replace. (figure 4-8)

- (1) Unscrew knob (1) from retainer (2).
- (2) Drill out rivet (3) and remove knob assembly from retainer (2). Drill out rivet (4) and remove retainer from door. (Refer to paragraph 3-9.a. for rivet removal instructions.)

NOTE

Anchor tab of knob assembly chain to side rivets on top retainers and bottom rivets on bottom retainers.

- (3) Position retainer (2) on door and install one rivet (4). (Refer to paragraph 3-9.a. for rivet installation instructions.)
- (4) Screw knob (1) into retainer (2) and into frame of emergency exit.
- (5) Position tab (5) of knob assembly chain over second rivet hole in retainer (2) and install rivet (3).

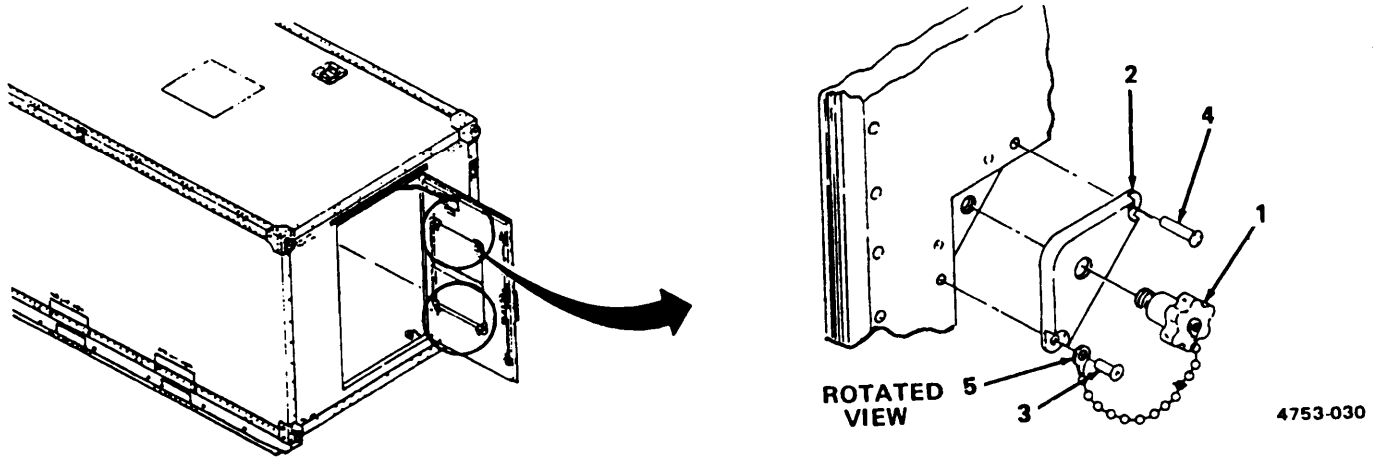


Figure 4-8. Door Knob Assembly Replacement.

4-17. Door Hinge Assemblies.

This task covers: Replace

INITIAL SETUP

<i>Tools</i>	<i>Materials/Parts</i>
General Mechanic's Automotive Tool Kit	Sealer (Item 29 or 30, Appendix D)
SC 5180 -90-CL-N26	Shims, SM-B-162197
Electronic Equipment Shelter Tool Kit TK-144/G	

Replace. (figure 4-9)

NOTE

The shelter door has four hinge assemblies. This procedure is typical for all four. Do not remove more than one hinge at a time.

- (1) Remove five bolts (1 and 2), five self-locking nuts (3) and five flat washers (4) and take hinge assembly (5) and shim(s) (6) off door.
- (2) Coat both sides of shim(s) (6) with sealer.
- (3) Position hinge assembly (5) and shim(s) (6) on door and fasten with two long bolts (2), three short bolts (1), five flat washers (4) and five self-locking nuts (3).
- (4) Check latch torque. Latch torque should be 15 foot-pounds (max) without RFI/EMI gasket, or 30 foot-pounds (max) with RFI/EMI gasket. Add or subtract shims (6) to achieve proper latch torque. Latch torque may also be adjusted by varying number of latch keeper shims (para 3-15).
- (5) Lubricate as required (para 3-1).

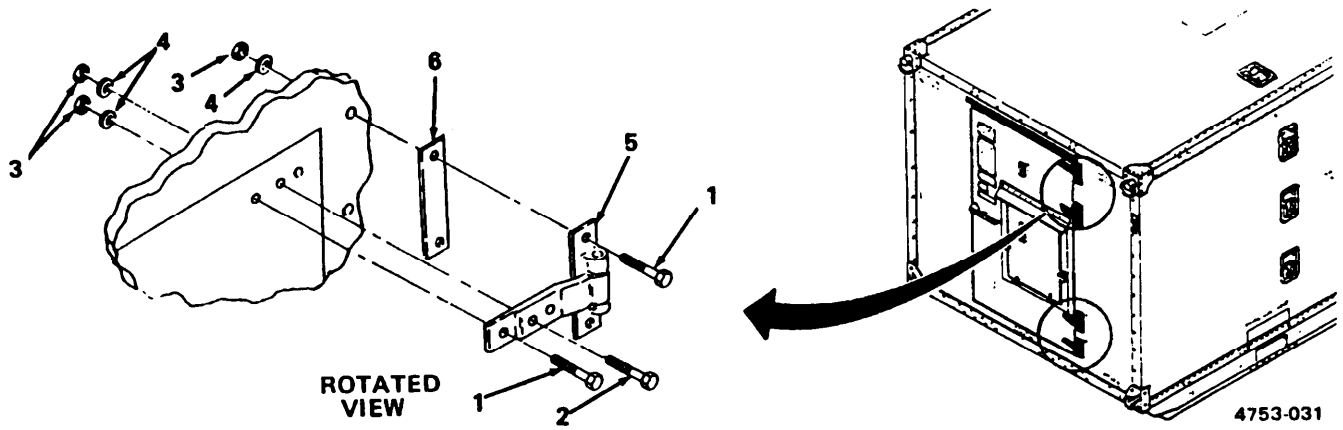


Figure 4-9. Door Hinge Assembly Replacement.

4-I8. Door Skin.

This task covers: Repair

INITIAL SETUP

Tools

General Safety Instructions

Electronic Equipment Shelter Tool Kit
TK-144/G
General Mechanic's Automotive Tool Kit
SC 5180-90-CL-N26
Blind Riveter

WARNING

Adhesives contain toxic solvents. Avoid eye and skin contact and breathing of vapors. Use in a well-ventilated area. Use protective goggles and gloves. Use in accordance with manufacturer's instructions.

Materials/Parts

Adhesive Kit (Item 6, Appendix D)
Rivets, Various
Gloves (Item 12, Appendix D)
Goggles (Item 38, Appendix D)

Drilling creates metal chips which may enter eyes and cause serious injury. Eye protection is required.

Repair.

NOTE

This procedure covers repair of door skin swelling and delamination. For patching of punctures, refer to paragraph 4-20.

The door skin is bonded to the underlayer with adhesive. The underlayer is solid wood in some areas and wood veneer over aluminum in other areas. Delamination occurs when unbroken skin pulls away from the underlayer.

- (1) Drill 1/4-inch deep holes through skin into underlayer, using a no. 20 drill bit. Space holes 1-1/2 inches apart along entire length of delaminated area.
- (2) Determine if subsurface is solid wood block or wood veneer over extruded aluminum.
- (3) Prepare adhesive by mixing base material and hardener in accordance with manufacturer's instructions. Use materials within one year from date of manufacture.
- (4) Apply adhesive between skin and underlayer.
- (5) Install screws in drilled holes where underlayer is solid wood block. Install rivets where underlayer is veneer over extruded aluminum. (Refer to paragraph 3-9.a for rivet installation instructions.)

4-19. RFI/EMI Components.

This task covers: Replace

INITIAL SETUP

Tools

Materials/Parts

As required

RFI filter, PN SM-C-450478

Replace. RFI/EMI component replacement is limited to replacement of the RFI filter (para 4-15).

4-20. Wall, Floor and Ceiling Panels.

This task covers: Repair

INITIAL SETUP

Tools

Electronic Equipment Shelter Tool Kit
TK-144/G
General Mechanic's Automotive Tool Kit
SC 5180-90-CL-N26
Blind Riveter

Materials/Parts (cont)

Sealer (item 29 or 30, Appendix D)
Cheesecloth (item 9 or 10, Appendix D)
Gloves (Item 12, Appendix D)
Goggles (Item 38, Appendix D)

Materials/Parts

Aluminum, Unpainted (Item 7 or 8, Appendix D)
Sandpaper, Grit Nos. 40,60 and 80
(Items 26, 27 and 28, Appendix D)
Solvent (Item 37, Appendix D)
Blind "Pop" Rivets, Various Sizes and
Types
Adhesive (Item 6, Appendix D)

General Safety Instructions

WARNING

Adhesives and solvents are flammable and toxic.
Keep away from heat and open flames. Avoid eye
and skin contact and breathing of vapors. Use in a
well-ventilated area. Use protective goggles and
gloves. Use in accordance with manufacturer's
instructions.

Repair. (figure 4-10)

CAUTION

Paint strippers can contaminate panel core, adhesive and sealer. Do not use paint strippers to remove paint.

RFI/EMI shielded shelters should not be operated until a permanent patch has been applied.

NOTE

The following procedures shall be used to repair small punctures that do not exceed 1/2-inch depth into foam core. All punctures must be patched immediately to prevent water intrusion and/or radiation leakage (shielded shelters). Dents without punctures do not require patching. However, if bare metal is exposed, touch up with paint (para 4-6).

Wall, ceiling and floor sandwich panels are alike in composition and construction. Repair procedures are the same for all sandwich panels.

- (1) Bend edges of puncture in below surface of unbroken face sheet. Do not allow broken edges to contact opposite face.
- (2) Remove loose fragments of foam and dust, using a vacuum, if necessary.

- (3) Cut a rectangular patch large enough to extend at least one inch beyond damaged area in all directions. Thoroughly degrease and clean patch within 72 hours before installation.
- (4) Center patch over damaged area, then lightly trace outline of patch on panel face.
- (5) Remove paint from panel face within marked outline by sanding or using a solvent. (Do not use paint stripper.) All traces of paint must be removed.

WARNING

Drilling creates metal chips which may enter eyes and cause serious injury. Eye protection is required.

- (6) Lay out rivet hole pattern around edge of patch. Rivet holes should be 1/4 to 1/2 inch in from edge of patch and one inch apart. Drill holes using a no. 11 or no. 12 drill.
- (7) Center patch over damaged area of panel.

NOTE

Drill two diagonally opposite corner holes first, then other two holes, then drill remaining holes.

- (8) Using drilled holes in patch as a guide, drill rivet holes in panel face sheet. Be careful not to drill through opposite face sheet. Insert a rivet in each hole as it is drilled to keep patch in place.
- (9) Remove patch and remove all burrs from drilled holes.
- (10) If puncture in panel is surrounded by extended cracks, drill a hole at the end of each crack, using a no. 30 drill, to keep crack from spreading.
- (11) Prepare adhesive by mixing base material and hardener in accordance with manufacturer's instructions. Use materials within one year from date of manufacture.
- (12) Prepare bonding surface of panel face sheet for bonding by sanding until oxide film is removed and bright surface is exposed.
- (13) Inject adhesive into puncture.
- (14) After adhesive has hardened, sand until adhesive is flush with surface of panel face.
- (15) Remove all contaminants (dirt, dust, oil, etc.) from bonding surfaces of patch and panel face, using a vacuum or clean, dry cloth. Wipe surfaces with clean cloth soaked in solvent and immediately wipe solvent from surface with clean cloth. Wear gloves to avoid contaminating surfaces with dirt, oil or fingerprints.
- (16) Apply thin, even layer of adhesive to bonding surfaces of panel face sheet and patch. Position patch in place with sheet fasteners.

4-20. Wall, Floor and Ceiling Panels (cont).

NOTE

When repairing an external face sheet, before installing rivets, inject sealer into drilled holes to prevent moisture from entering panel.


(17) Rivet patch to face sheet. (Refer to para 3-9.a for rivet installation instructions.)

(18) Wipe excess adhesive from surface of repaired area. Do not use solvent.

(19) Allow adhesive to dry.

(20) Coat edges of patch and rivet heads with sealer.

(21) Repaint as required (para 4-6).

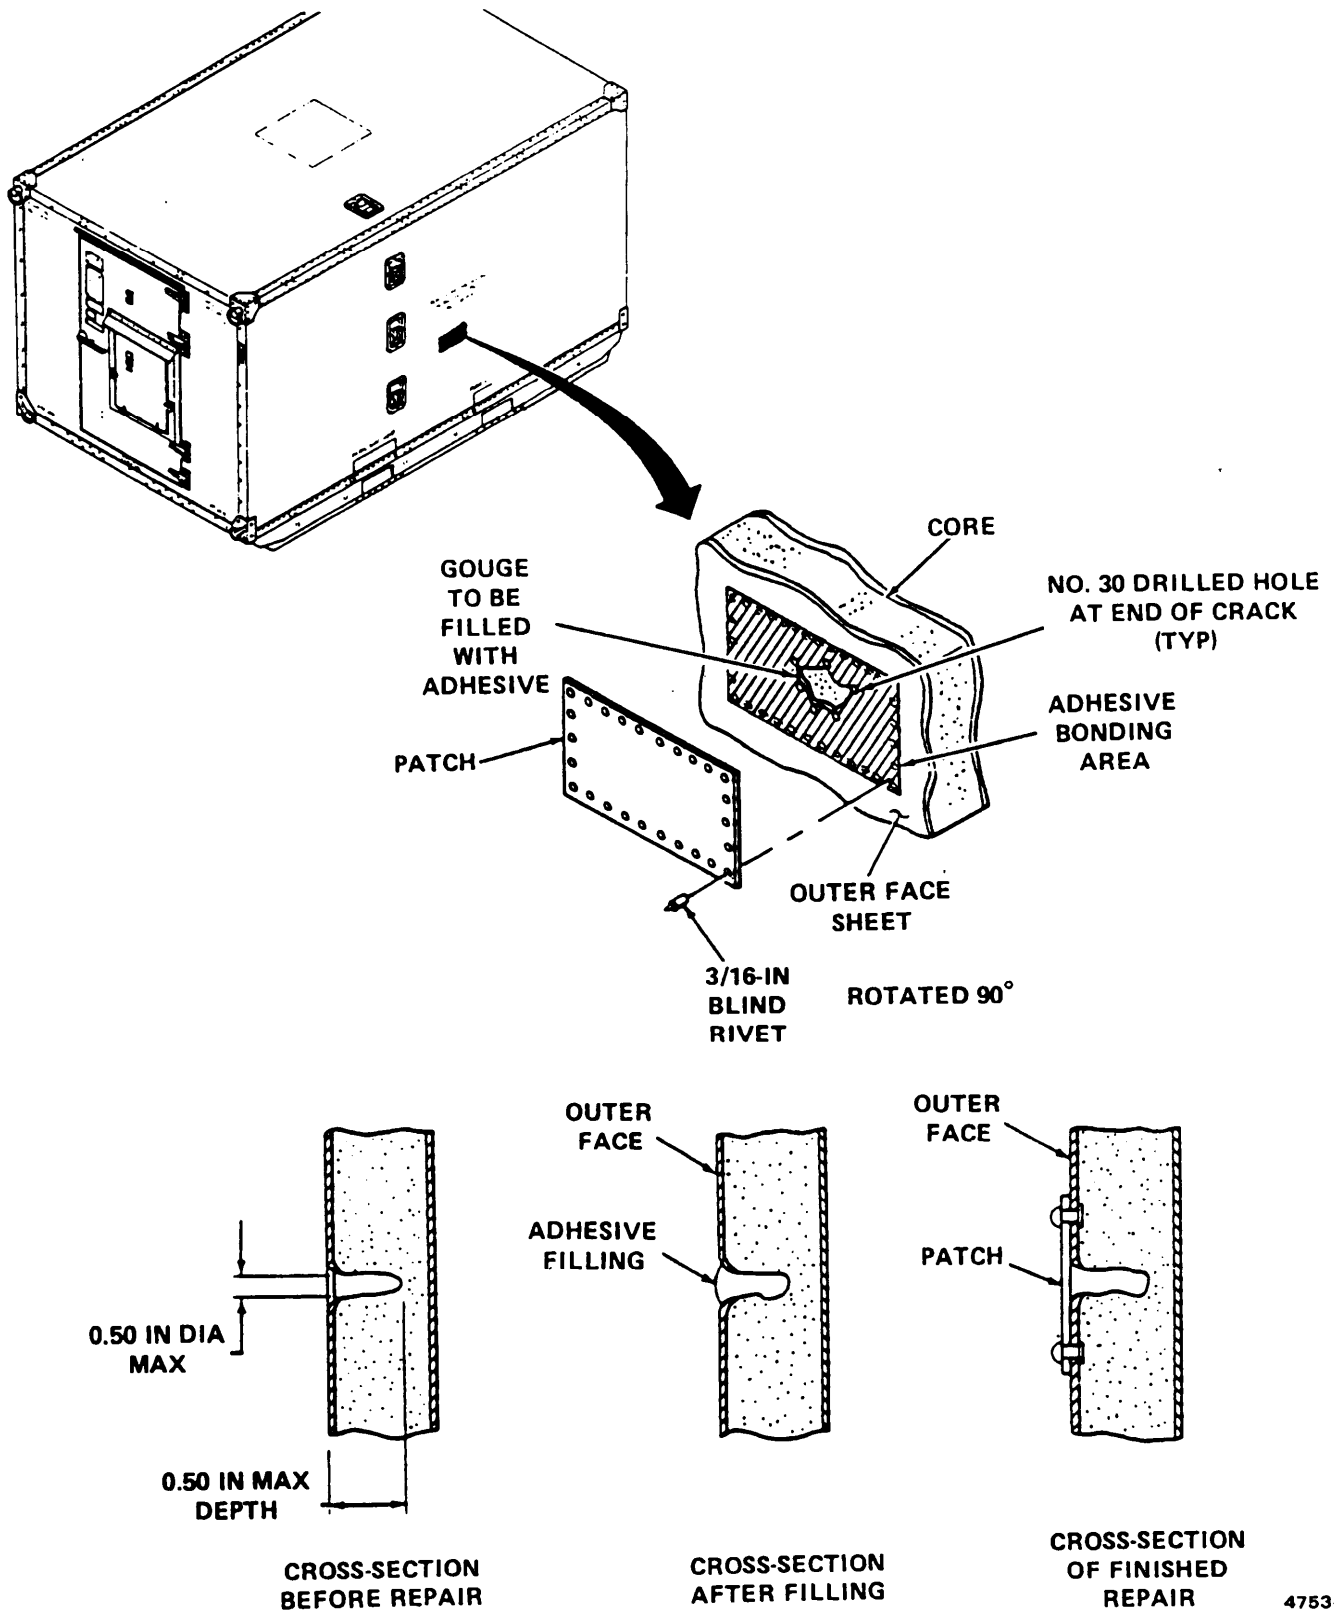

4753-035

Figure 4-10. Panel Repair

CHAPTER 5

GENERAL SUPPORT MAINTENANCE INSTRUCTIONS

Subject	Section	Page
Repair Parts, Special Tools, TMDE and Support Equipment	I	5-1
General Support Maintenance Procedures	II	5-1

Section I. REPAIR PARTS, SPECIAL TOOLS, TMDE AND SUPPORT EQUIPMENT

Subject	Para	Page
Common Tools	5-1	5-1
Special Tools, TMDE and Support Equipment	5-2	5-1
Repair Parts	5-3	5-1

5-1. **Common Tools.** A complete list of common tools and tool kits is given in Section III of Appendix B, Maintenance Allocation.

5-2. **Special Tools, TMDE and Support Equipment.** There are no special tools or equipment needed to maintain the shelters.

5-3. **Repair Parts.** Repair parts for general support maintenance of the shelters are listed and illustrated in TM 10-5411-206-24P.

Section II. GENERAL SUPPORT MAINTENANCE PROCEDURES

Subject	Para	Page
General	5-4	5-1
Surface Preparation, Priming and Painting	5-5	5-1
Door Assembly	5-6	5-2
Towing Eye Assemblies	5-7	5-4
Lifting Eye Assemblies	5-8	5-6
RFI/EMI Shielding Gaskets	5-9	5-8
Wall and Ceiling Panels	5-10	5-10
Skid Assemblies and Mounting Brackets	5-11	5-14

5-4. **General.** This section contains maintenance procedures which are the responsibility of general support maintenance, as authorized by the Maintenance Allocation Chart (appendix B). The general maintenance information given for unit level maintenance also applies to intermediate general support level maintenance. This information is contained in paragraph 3-8.

5-5. **Surface preparation, Priming and Painting.** All bare metal shall be painted to prevent corrosion. Touch up small dents and chips. Repaired sections of panels must be prepared with a corrosion protection primer before painting. Do not attempt to repaint large areas such as complete exterior interior or ceiling. Detailed priming and painting instructions can be found in TM 43-0139.

5-6. **Door Assembly.**

This task covers: Replace

INITIAL SETUP

<i>Tools</i>	<i>Personnel Required</i>
General Mechanic's Automotive Tool Kit SC 5180 -90-CL-N26	Two
Electronic Equipment Shelter Tool Kit TK-144/G	Equipment Condition
<i>Materials/Parts</i>	Door brace assembly removed (para 3-11).
Sealer (Item 29 or 30, Appendix D)	

Replace. (figure 5-1)

NOTE

One person should support door assembly while second person removes and installs hardware.

- (1) Remove two bolts (1), two self-locking nuts (2) and two flat washers (3) securing each hinge (4) to shelter wall.
- (2) Push door assembly (5) out of shelter. Remove hinge shims (6).
- (3) Position shim(s) (6) against underside of each door hinge (4) and insert two bolts (1) through each hinge and shim(s).
- (4) Position door assembly (5) in shelter cutout and insert bolts (1) through mounting holes in shelter wall.
- (5) Install one flat washer (3) and one self-locking nut (2) on each bolt (1).
- (6) Check latch torque. Latch torque should be 15 foot-pounds (30 foot-pounds with RFI/EMI gasket). Add or subtract hinge shims (6) to achieve proper torque.

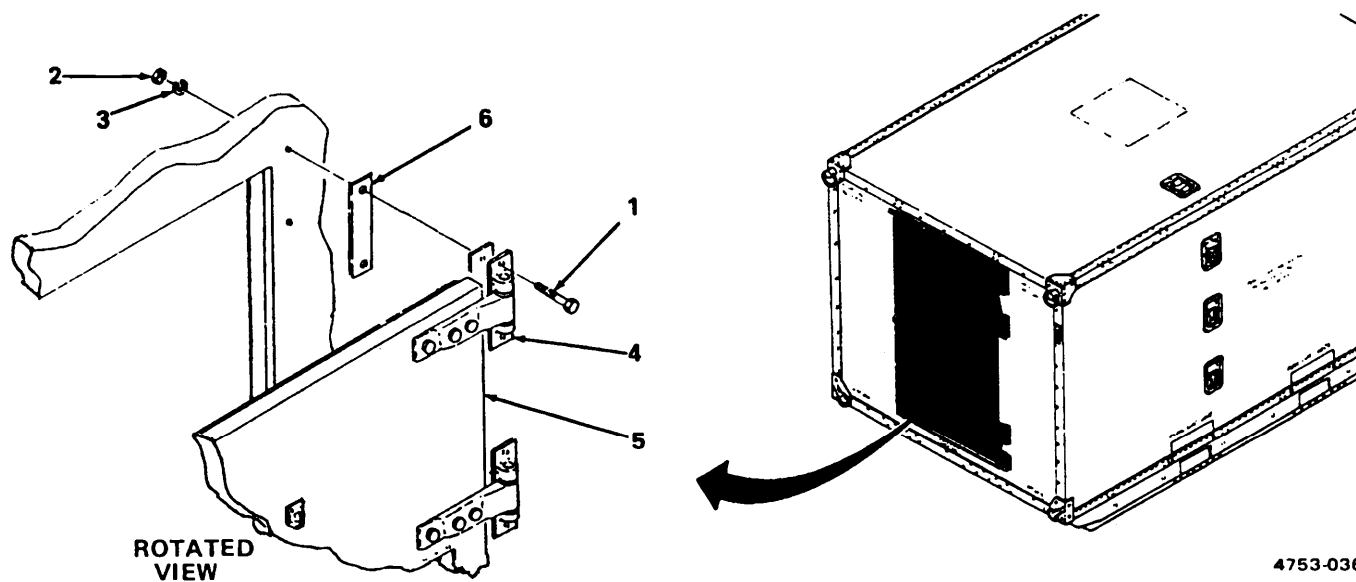


Figure 5-1. Door Assembly Replacement.

NOTE

FOLLOW-ON MAINTENANCE: Install door brace assembly (para 3-11).

5-7. Towing Eye Assemblies.

This task covers: a. Remove b. Disassemble c. Assemble d. Install

INITIAL SETUP*Tools*

General Mechanics Automotive Tool Kit
 SC 5180 -90-CL-N26
 Electronic Equipment Shelter Tool Kit TK-144/G

Equipment Condition

Skid assembly and mounting bracket removed
 (para 5-11).

Materials/Parts

Sealer (Item 29 or 30, Appendix D)

NOTE

The shelter has one towing eye assembly at each bottom corner. This procedure is typical for all four.

a. *Remove. (figure 5-2)*

- (1) Remove five socket head screws (1), two cap screws (2), two flat washers (3) and two lockwashers (4) and remove towing eye assembly (5 through 8).
- (2) Remove and retain shims (9 and 10).
- (3) Inspect condition of rivnuts (11) and replace if necessary (para 3-9.b).

b. *Disassemble (figure 5-2)*

Remove bolt (5) and self-locking nut (6) and take towing eye (7) off fitting (8).

c. *Assemble (figure 5-2)*

Position towing eye (7) on fitting (8) and fasten with bolt (5) and self-locking nut (6). Make sure bolt head is on top and nut on bottom, as shown in figure 5-2.

d. *Install. (figure 5-2)*

- (1) Coat both sides of shims (9 and 10) and entire inside of fitting (8) with sealer.
- (2) Position shims (9 and 10) against inside of towing eye fitting (8) so that mounting holes line up.
- (3) Position towing eye assembly (5 through 8) on shelter corner so that eye (8) is on front or rear of shelter, as applicable.

- (4) Install five socket head screws (1) in side and bottom mounting locations.
- (5) Install two cap screws (2), two lockwashers (4) and two flat washers (3) in ring side mounting locations.
- (6) Apply a bead of sealer around edge of fitting (8).
- (7) Lubricate as required (para 3-1).

NOTE

FOLLOW-ON MAINTENANCE: Install skid assembly and mounting bracket (para 5-11).

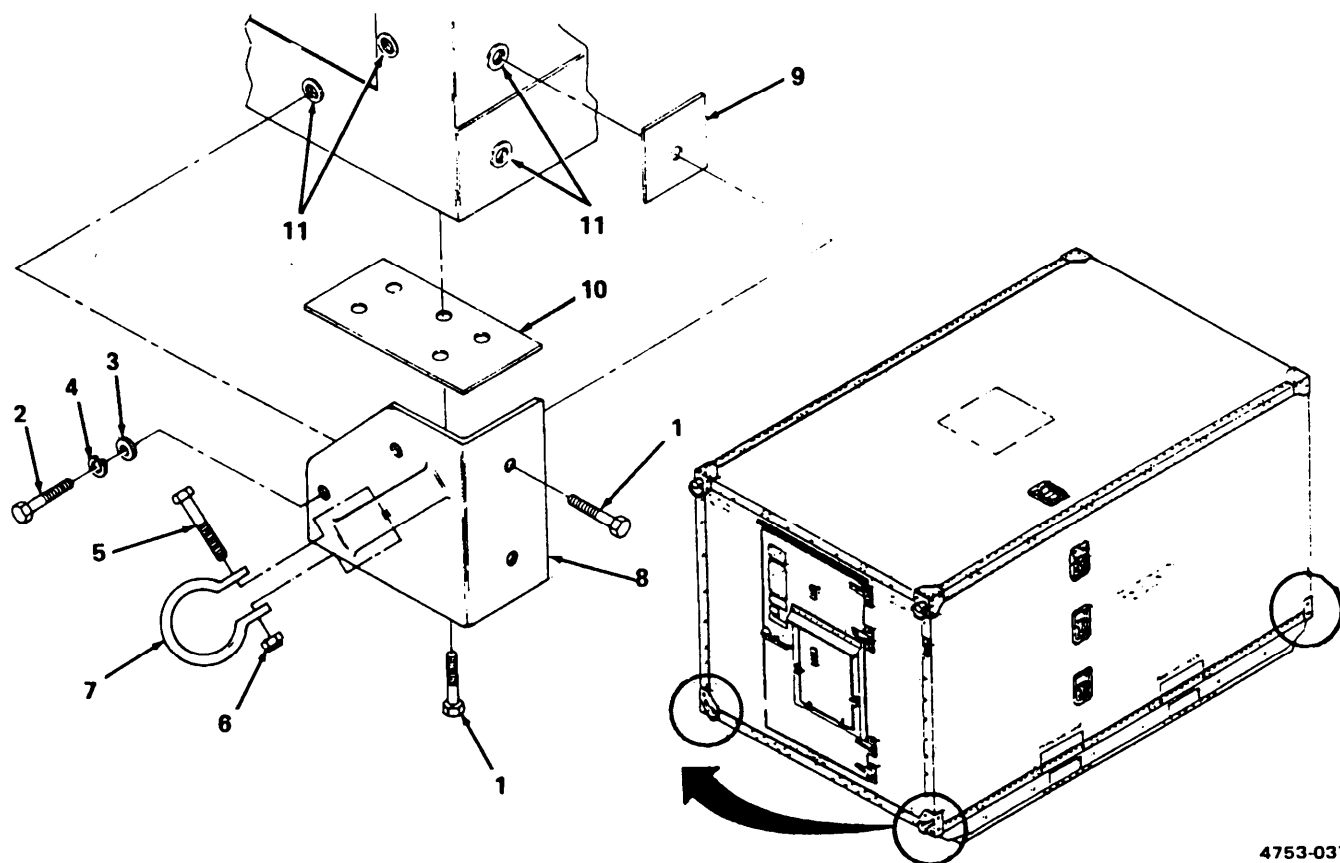


Figure 5-2. Towing Eye Assembly Repair and Replacement.

5-8. Lifting Eye Assemblies.

This task covers: a. Remove b. Disassemble c. Assemble d. Install

INITIAL SETUP

Tools

General Mechanic's Automotive Tool Kit
 SC 5180 -90-CL-N26
 Electronic Equipment Shelter Tool Kit TK-144/G

Materials/Parts

Sealer (Item 29 or 30, Appendix D)

NOTE

The shelter has one lifting eye assembly at each top corner. This procedure is typical for all four lifting eye assemblies.

a. *Remove. (figure 5-3)*

- (1) Remove four cap screws (1), four flat washers (2), four lockwashers (3) and 11 socket head screws (4 and 5) and remove lifting eye assembly (6 through 10).
- (2) Remove and retain shims (11 and 12).
- (3) Inspect condition of rivnuts (13) and replace if necessary (para 3-9.b).

b. *Disassemble. (figure 5-3)*

- (1) Remove setscrew (6).
- (2) Unscrew and remove swivel pin (7) from ring assembly (8).
- (3) Pull ring assembly (8) out of casting (9) and remove spacer (10).


c. *Assemble. (figure 5-3)*

- (1) Position spacer (10) on casting (9) and insert threaded end of ring assembly (8).
- (2) Thread swivel pin (7) onto ring assembly (8) inside casting (9). Secure in place with setscrew (6).
- (3) Apply lubricant liberally to interior surfaces of swivel pin (7) and ring assembly (8).

d. *Install. (figure 5-3)*

- (1) Coat both sides of shims (11 and 12) and entire inside surface of casting (9) (except for area around swivel pin (7)) with sealer.
- (2) Position shims (11 and 12) against inside of casting (9) so that mounting holes line up.

- (3) Install four cap screws (1), four lockwashers (3) and four flat washers (2) in ring side of lifting eye assembly.
- (4) Install nine long (1-1/8 in.) socket head screws (4) and two short (1 in.) socket head screws (5) in top and side of lifting eye assembly.
- (5) Apply a bead of sealer around edge of casting (9).
- (6) Lubricate as required (para 3-1).

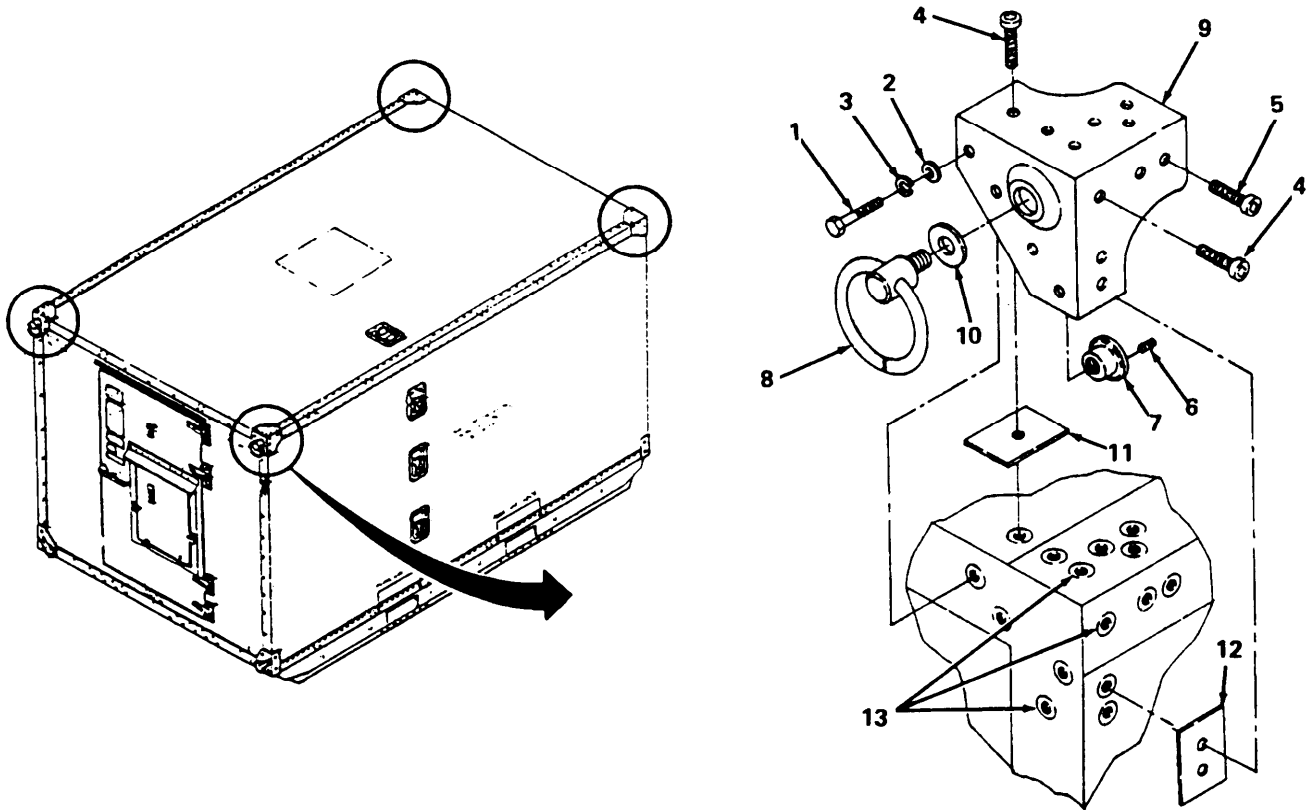

4753-038

Figure 5-3. Lifting Eye Assembly Repair and Replacement.

5-9. RFI/EMI Shielding Gaskets.

This task covers: Replace

INITIAL SETUP*Tools*

General Mechanics Automotive Tool Kit
SC 5180-90-CL-N26
Electronic Equipment Shelter Tool Kit
TK-144/G

Materials/Parts

Solvent (Item 37, Appendix D)
Sealer (Item 29 or 30, Appendix D)
Gloves (Item 12, Appendix D)
Primer (Item 23, Appendix D)
Gasket
Goggles (Item 38, Appendix D)

*General Safety Instructions***WARNING**

Solvents and sealers are flammable and toxic. Keep away from heat and open flames. Avoid skin and eye contact and breathing of vapors. Use in a well-ventilated area. Use protective goggles and gloves. Use in accordance with manufacturer's instructions.

Replace. (figure 5-4)

NOTE

In shelters with RFI/EMI shielding, both outer door and inner door have shielding gaskets installed around inside edge. Replacement procedures are the same for both.

- (1) Remove gasket and scrape channel clean.
- (2) Remove residue of paint or sealer with solvent.
- (3) Cut new gasket to required length (complete length of channel) plus 2-1/2 inches.

NOTE


Sealer must be applied between 30 minutes and eight hours after application of primer.

- (4) Apply primer, then sealer, evenly to sides and bottom of gasket channel to insure a continuous bond.
- (5) Immediately after applying sealer, press new gasket into place so that ends of gasket meet on hinged side of door.

NOTE

Make gasket splice approximately midway up hinged side of door.

- (6) Pull back wire mesh shielding on one end of gasket, exposing sponge core.
- (7) Cut off 2-1/4 inches of exposed core. Do not cut wire mesh shielding.
- (8) Join ends of sponge core.
- (9) Roll wire mesh shielding over joined ends.

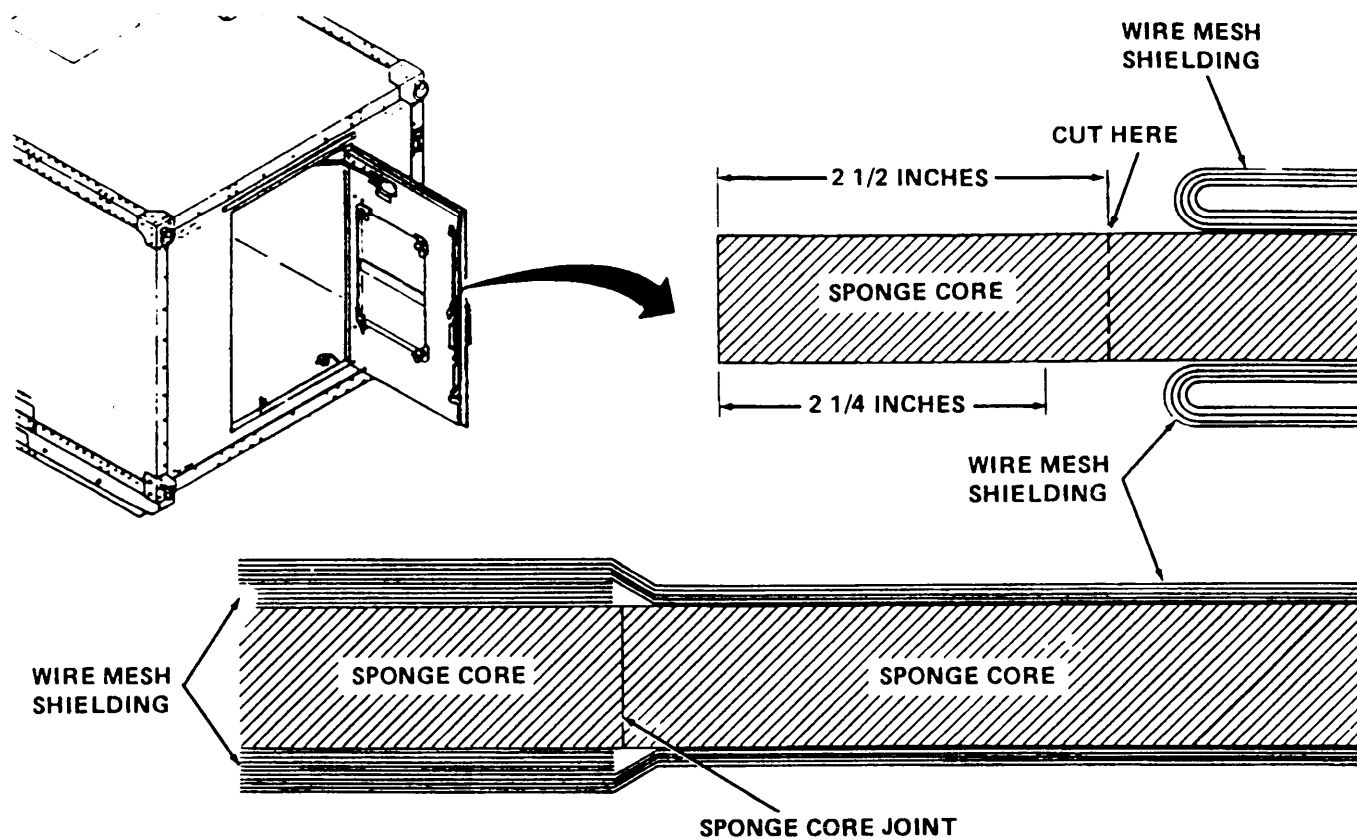

4753-039

Figure 5-4. RFI/EMI Shielding Gasket Replacement.

5-10. Wall and Ceiling Panels.

This task covers: Repair

INITIAL SETUP

Tools

General Mechanics Automotive Tool Kit
 SC 5180 -90-CL-N26
 Electronic Equipment Shelter Tool Kit TK-144/G
 Blind Riveter

Materials/Parts (cont)

Cheesecloth (item 9 or 10, Appendix D)
 Gloves (Item 12, Appendix D)
 Goggles (Item 38, Appendix D)

General Safety Instructions

Materials/Parts

Aluminum, Unpainted (Item 7 or 8, Appendix D)
 Sandpaper, Grit Nos. 40, 60 and 80
 (Items 26, 27 and 28, Appendix D)
 Solvent (Item 37, Appendix D)
 Insulation, Rigid Urethane Foam (Item 15,
 Appendix D)
 Blind "Pop" Rivets, Various Sizes and Types
 Adhesive (Items 2, 3, 4 or 5, Appendix D)
 Sealer (Item 29 or 30, Appendix D)

WARNING

Adhesives and solvents are flammable and toxic. Keep away from heat and open flames. Avoid eye and skin contact and breathing of vapors. Use in a well-ventilated area. Use protective goggles and gloves. Use in accordance with manufacturer's instructions.

Drilling, sawing, and filing create metal chips which may enter eyes and cause serious injury. Eye protection is required.

Repair. (figure 5-5)

Caution

Paint strippers can contaminate panel core, adhesive and sealer. Do not use paint strippers to remove paint.

RFI/EMI shielded shelters should not be operated until a permanent patch has been applied.

NOTE

The following procedures shall be used to repair large punctures with foam core damage. All punctures must be patched immediately to prevent water intrusion and/or radiation leakage (shielded shelters). Dents without punctures do not require patching. However, if bare metal is exposed, touch up with paint (para 5-5).

Wall and ceiling sandwich panels are alike in composition and construction. Repair procedures are the same for both. If floor panel damage is too extensive to patch as described in paragraph 4-10, refer the shelter to higher maintenance level.

- (1) Cut a rectangular patch large enough to encompass damaged area on face sheet. Patch material must be same thickness as panel face sheet.
- (2) Using patch as a template, mark rectangle on face sheet covering damaged area. This will ensure that patch will fit snugly in face sheet cutout when patch is installed.
- (3) Cut out damaged face sheet within rectangle, using a router bit chucked in a 1/4-inch drill, a fine-tooth keyhole type hacksaw, or a circular saw.
- (4) Cut and remove core material to opposite face sheet using a knife.
- (5) If both sides of panel are damaged, repeat steps (1) through (3) for opposite side of panel. Second cutout should be identical to and directly opposite first cutout.
- (6) File cutout edges smooth, using fine cut, half round file, or rotary file chucked in 1/4-inch drill.
- (7) Remove loose fragments of foam, dust and metal. Use a vacuum, if necessary.
- (8) Remove paint from panel face around each cutout for a distance of 1-1/2 inches (up to two inches for very large cutouts). Paint may be sanded off or removed with solvent. All traces of paint must be removed.
- (9) If only one face sheet has been cut out, clean bonding (interior) surface of opposite face sheet until smooth.

NOTE

If cutouts have been made in both sides of panel, steps (10) through (15), (17), (18) and (21) through (25) apply to both face sheets.

- (10) Cut a doubler for patch. Make doubler one inch larger all around that cutout (up to two inches for very large cutouts).
- (11) Lay out rivet hole pattern in patch and doubler. Rivet holes should be 1/4 to 1/2 inch from edge and one inch apart. (Hole spacing may be increased to two inches when distance between two corner holes exceeds 20 inches.) Drill holes using a no. 11 or no. 12 drill (no. 12 or no. 30 for large patches). Remove all metal chips and burrs from drilled holes.
- (12) Center patch on doubler and drill rivet holes in doubler, using drilled holes in patch as a template. Secure patch to doubler by temporarily inserting rivets.
- (13) Center doubler (with patch temporarily fastened) over cutout in panel, making sure patch fits snugly and flush in cutout.

NOTE

Drill two diagonally opposite corner holes first, then other two corner holes, then drill remaining holes.

5-10. Wall and Ceiling Panels (cont).

- (14) Drill rivet holes in panel face sheet, using holes drilled in doubler as a template. Use drill and pin as a stop by placing drill inside pin and setting drill in chuck so that 7/16 to 9/16 inch of drill is exposed when pin is against chuck jaws. Temporarily insert a rivet in each hole as it is drilled to keep patch and doubler from moving.
- (15) Remove doubler and patch. Remove all metal chips and remove burrs from drilled holes.

CAUTION


When machining foam core, be careful not to crush foam, since this results in water absorption. Do not use a plane to machine foam.

- (16) Cut section of new foam core material to fit snugly in core cavity. Core material must be flush with inside of both panel faces when installed. Use a single piece of foam.
- (17) Prepare bonding surfaces of face sheet, patch and doubler for bonding by sanding until oxide film is removed and bright surface is exposed.
- (18) Wipe surfaces with clean cloth soaked in solvent. Immediately wipe solvent from surface with clean cloth. Wear gloves to avoid contaminating surfaces with dirt, oil or fingerprints.
- (19) Prepare adhesive by mixing base material and hardener in accordance with manufacturer's instructions. Use materials within one year from date of manufacture.
- (20) Apply adhesive liberally to all surfaces of new core material and cavity and position core material in cavity.
- (21) Apply a thin, even layer of adhesive to bonding surfaces of face sheet, patch and doubler. Position patch in place on doubler with sheet fasteners.

NOTE

When repairing an external face sheet, before installing rivets, inject sealer into drilled holes to prevent moisture from entering panels.

- (22) Rivet patch to doubler and doubler to face sheet. (Refer to paragraph 3-9.a for rivet installation instructions.)
- (23) Wipe excess adhesive from outer surfaces of repaired area. Do not use solvent to remove adhesive.
- (24) Allow adhesive to dry.
- (25) Coat edges of doubler and rivet heads with sealer,
- (26) Touch up with paint as required (para 5-5).

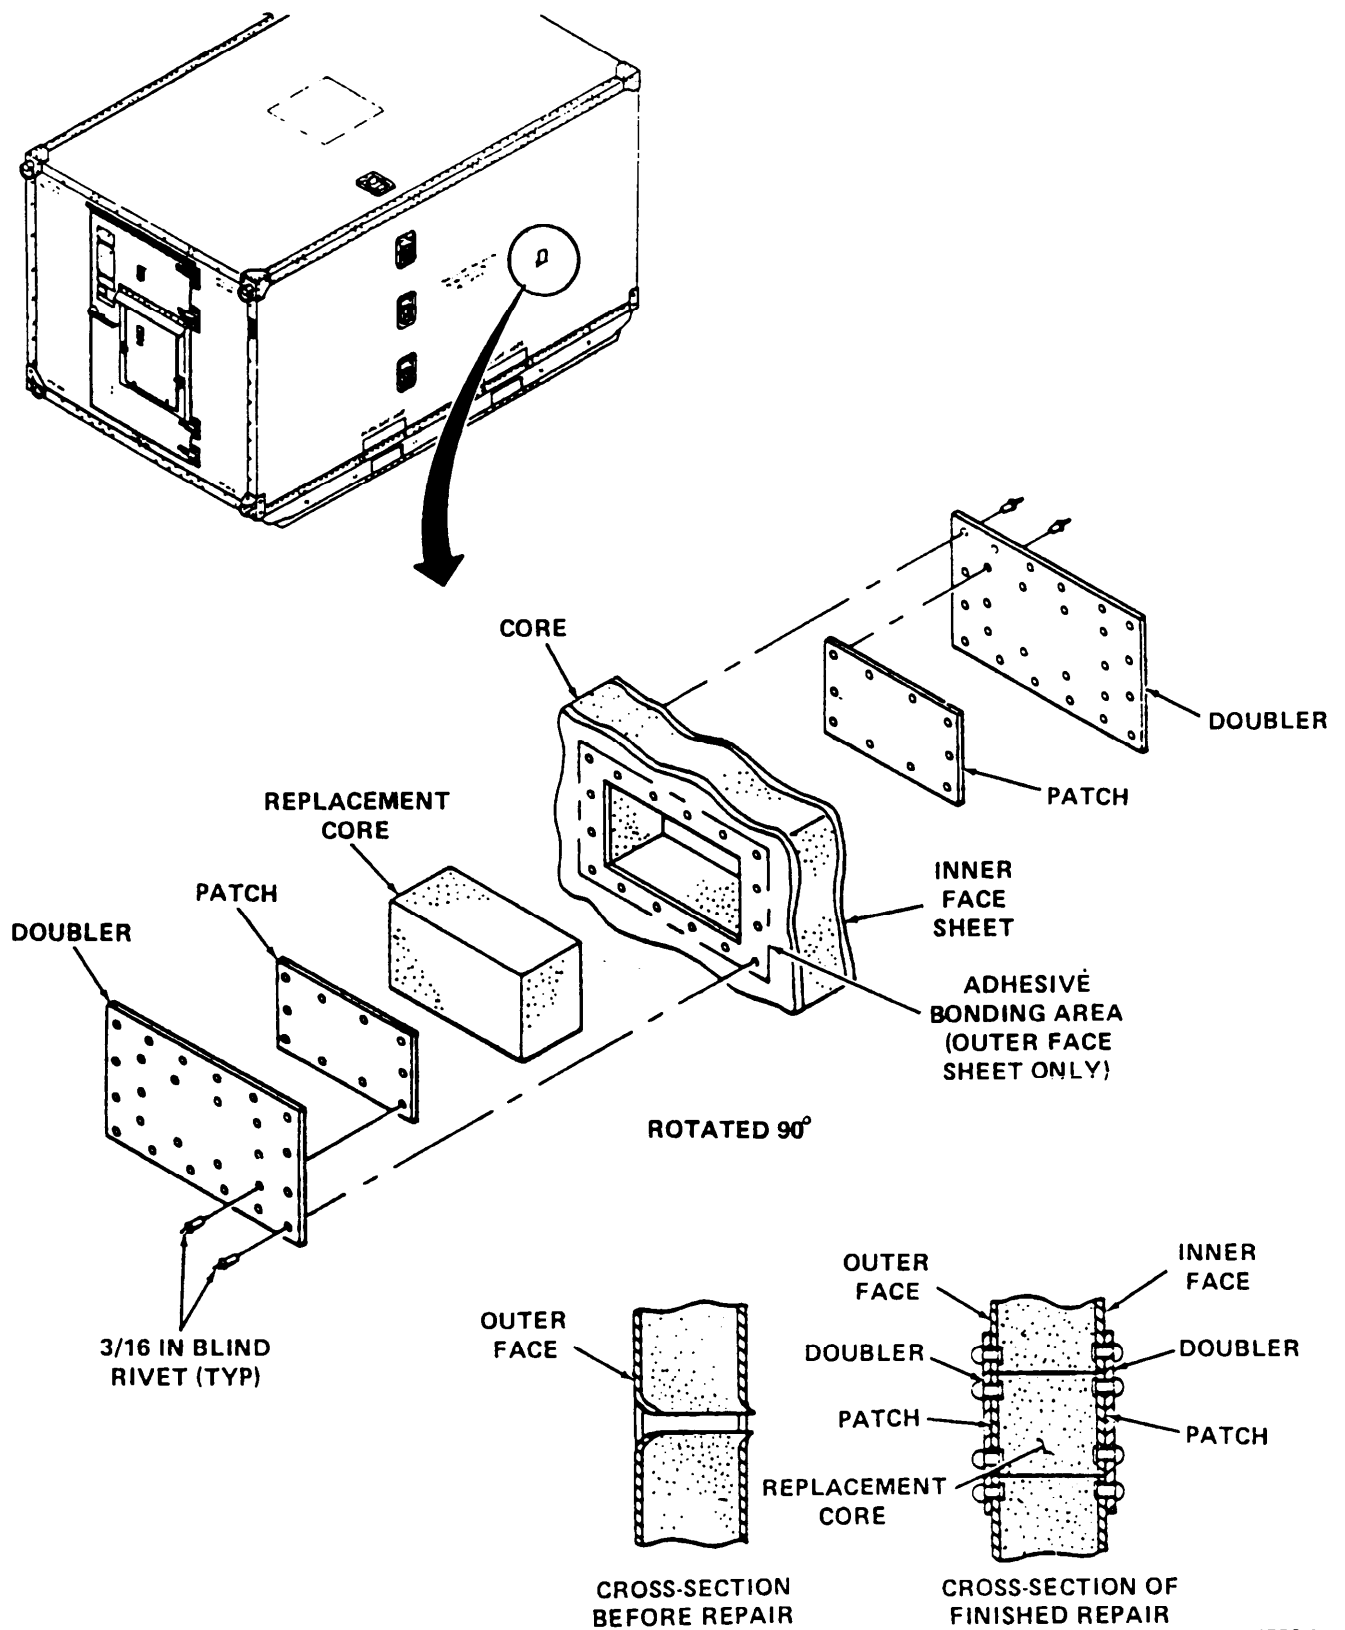

4753-040

Figure 5-5. Panel Repair.

5-11. Skid Assemblies and Mounting Brackets.

This task covers: Replace

INITIAL SETUP

<i>Tools</i>	<i>Materials/Parts</i>
General Mechanic's Automotive Tool Kit SC 5180-90-CL-N26	Sealer (Item 29 or 30, Appendix D) Rivnuts, Various
Electronic Equipment Shelter Tool Kit TK-144/G	<i>Personnel Required</i>
	Four

Replace. (figure 5-6)

NOTE

The shelter has three skid assemblies and three mounting brackets. The procedure is the same for all three, except where noted.

- (1) Lift shelter and load it onto blocks high enough to allow ample clearance between skid assemblies and floor for hardware removal and installation. (Refer to paragraph 3-5 for lifting and loading instructions.)
- (2) Remove six hex head bolts (1), six hex nuts (2) and twelve flat washers (3) and remove skid assembly (4) from mounting bracket (5).
- (3) Remove eight socket head screws (6), 48 hex head screws (7 and 8), four flat washers (9) and four lockwashers (10) and remove mounting bracket (5) from shelter floor.

NOTE

Shims (12 and 13) are only used with center mounted skid mounting bracket.


- (4) Remove shims (11 through 13). Record number of shims (11) removed.
- (5) Inspect rivnuts and replace if necessary (para 3-9.b).
- (6) Position shims (11) on ends of mounting bracket (5). Use same number of shims removed (step (4)).

NOTE

Shims (12 and 13) are only used with center mounted skid mounting bracket.

- (7) Position one shim (12) on each end of mounting bracket (5) on top of shims (11). Place shim (13) on mounting bracket. Make sure all mounting holes line up.

- (8) Coat exposed side of shim (13) (the side that will mate with shelter floor) with sealer.
- (9) Position mounting bracket (5), together with all shims, on shelter bottom.
- (10) Install four hex head screws (7), with one lockwasher (10) and one flat washer (9) each, in end pair of mounting holes at each end of mounting bracket (5). Install eight socket head screws (6) and 44 hex head screws (8) in remaining mounting holes.
- (11) If required, replace shelter on ground (para 3-5).

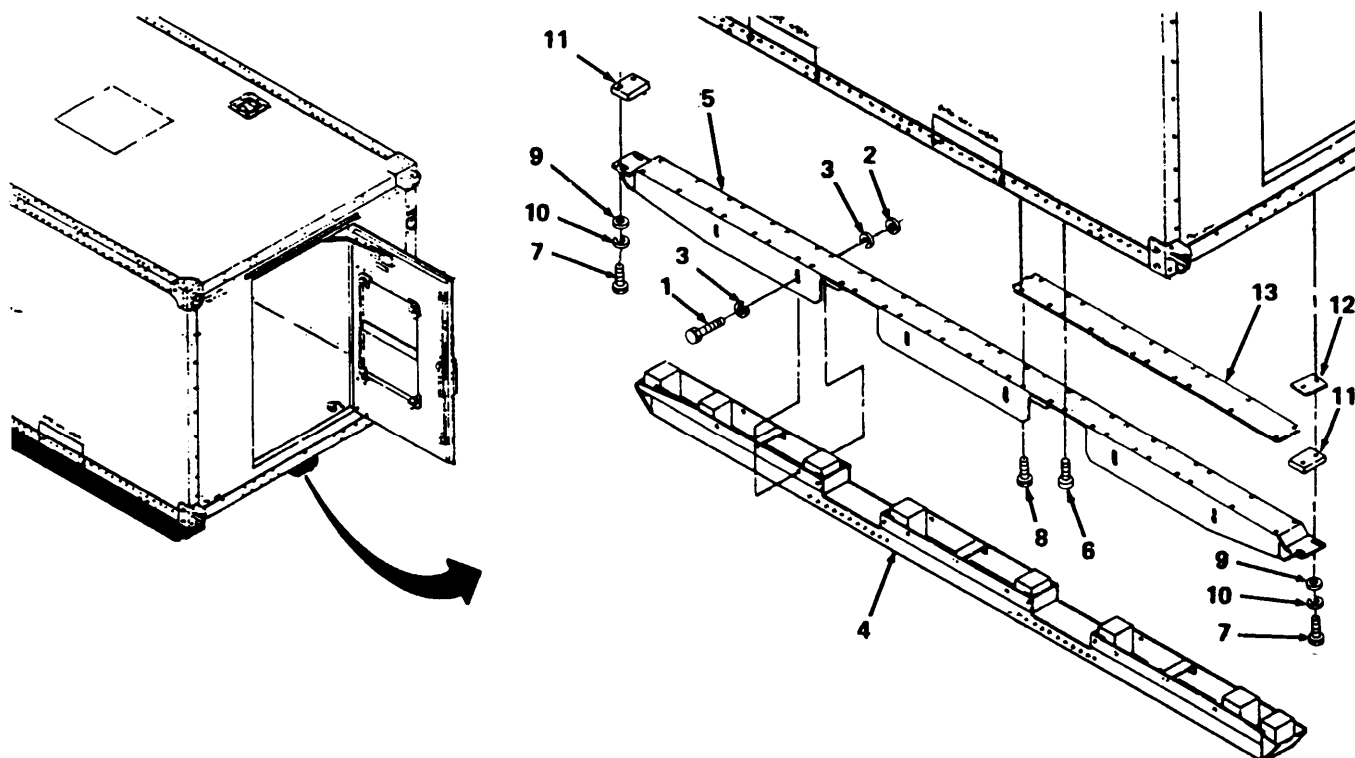

4753-041

Figure 5-6. Skid Assembly and Mounting Bracket Replacement.

APPENDIX A

REFERENCES

A-1. **Scope.** This appendix lists all forms, military specifications, technical manuals and miscellaneous publications referenced in this manual.

A-2. **Forms and Records.**

Recommended Changes to Publications and Blank Forms	DA Form 2028
Recommended Changes to Equipment Technical Publications	DA Form 2028-2
Equipment Inspection and Maintenance Worksheet	DA Form 2404
Report of item Discrepancy	SF364
Product Quality Deficiency Report	SF368

A-3. **Department of the Army Pamphlets.**

The Army Maintenance Management System (TAMMS)	DA Pam 738-750
--	----------------

A-4. **Military Specifications.**

Cloth, Cheesecloth, Cotton, Bleached and Unbleached	CCC-C-440
Coating, Epoxy, Polyamide	MIL-C-22750
Coating, Aliphatic, Polyurethane, Chemical Agent Resistant	MIL-C-46168
Lubricant, Solid Film, Air Drying, Corrosion Inhibiting	MIL-L-23398
Marking of Electronic Items	MIL-M-13231
Sealing Compound, Temperature-Resistant, Integral Fuel Tank and Fuel Cell Cavities, High Adhesion Sealant	MIL-S-8802
Silicone Compound, NATO Code Number S-736	MIL-S-22473
Aluminum Alloy, Bar, Rod, Shapes, Tube and wire, Extruded	QQ-A-200/8
Aluminum Alloy 6061, Plate and Sheet	QQ-A-250/11
Thinner, Synthetic Resin, Enamels	TT-T-306
Toluene, Technical Grade	TT-T-548

A-5. **Technical Manuals and Bulletins.**

Loading of S-280()/G Shelters in Container ANSI/ISO Type 1AA.	TB 11-5400-200-14
Repair Parts and Special Tools List for Shelter, Electrical Equipment S-280 B/G and S-280 B/G (Shielded)	TM 10-5411-206-24P
Painting instructions for Field Use	TM 43-0139
Destruction of Army Materiel to Prevent Enemy Use	TM 750-244-3

APPENDIX B

MAINTENANCE ALLOCATION CHART

SECTION I. INTRODUCTION

B-1. The Army Maintenance System MAC

This introduction provides a general explanation of all maintenance and repair functions authorized at the two maintenance levels under the Two-Level Maintenance System concept.

This MAC (immediately following the introduction) designates overall authority and responsibility for the performance of maintenance functions on the identified end item or component. The application of the maintenance functions to the end item or component shall be consistent with the capacities and capabilities of the designated maintenance levels, which are shown on the MAC in column (4) as:

Field - includes two columns, Unit maintenance and Direct Support maintenance. The Unit maintenance column is divided again into two more subcolumns, C for Operator or Crew and O for Unit Maintenance.

Sustainment – includes two subcolumns, General Support (H) and Depot (D).

The tools and test equipment requirements (immediately following the MAC) list the tools and test equipment (both special tools and common tool sets) required for each maintenance function as referenced from the MAC.

The remarks (immediately following the tools and test equipment requirements) contain supplemental instructions and explanatory notes for a particular maintenance function.

B-2. Maintenance Functions

Maintenance functions are limited to and defined as follows:

1. **Inspect.** To determine the serviceability of an item by comparing its physical, mechanical, and/or electrical characteristics with established standards through examination (e.g., by sight, sound, or feel.) This includes scheduled inspection and gagings and evaluation of cannon tubes.
2. **Test.** To verify serviceability by measuring the mechanical, pneumatic, hydraulic, or electrical characteristics of an item and comparing those characteristics with prescribed standards on a scheduled basis, i.e., load testing of lift devices and hydrostatic testing of pressure hoses.
3. **Service.** Operations required periodically to keep an item in proper operating condition, e.g., to clean (includes decontaminate, when required), to preserve, to drain, to paint, or to replenish fuel, lubricants, chemical fluids, or gases. This includes scheduled exercising and purging of recoil mechanisms. The following are examples of service functions:
 - a. **Unpack.** To remove from packing box for service or when required for the performance of maintenance operations.

- b. Repack. To return item to packing box after service and other maintenance operations.
 - c. Clean. To rid the item of contamination.
 - d. Touch up. To spot paint scratched or blistered surfaces.
 - e. Mark. To restore obliterated identification.
- 4. Adjust. To maintain or regulate, within prescribed limits, by bringing into proper or exact position, or by setting the operating characteristics to specified parameters.
 - 5. Align. To adjust specified variable elements of an item to bring about optimum or desired performance.
 - 6. Calibrate. To determine and cause corrections to be made, or to be adjusted on instruments of test, measuring, and diagnostic equipment used in precision measurement. Consists of comparisons of two instruments, one of which is a certified standard of known accuracy, to detect and adjust any discrepancy in the accuracy of the instrument being compared.
 - 7. Remove/Install. To remove and install the same item when required to perform service or other maintenance functions. Install may be the act of emplacing, seating, or fixing into position a spare, repair part, or module (component or assembly) in a manner to allow the proper functioning of an equipment or system.
 - 8. Paint. To prepare and spray color coats of paint so that the ammunition can be identified and protected. The color indicating primary use is applied, preferably, to the entire exterior surface as the background color of the item. Other markings are to be repainted as original so as to retain proper ammunition identification.
 - 9. Replace. To remove an unserviceable item and install a serviceable counterpart in its place. "Replace" is authorized by the MAC and assigned maintenance level is shown as the third position code of the Source, Maintenance and Recoverability (SMR) code.
 - 10. Repair. The application of maintenance services, including fault location/troubleshooting, removal/installation, disassembly/assembly procedures and maintenance actions to identify troubles and restore serviceability to an item by correcting specific damage, fault, malfunction, or failure in a part, subassembly, module (component or assembly), end item, or system.

NOTE

The following definitions are applicable to the “repair” maintenance function: Services. Inspect, test, service, adjust, align, calibrate, and/or replace.

Fault location/troubleshooting. The process of investigating and detecting the cause of equipment malfunctioning; the act of isolating a fault within a system or Unit Under Test (UUT).

Disassembly/assembly. The step-by-step breakdown (taking apart) of a spare/functional group coded item to the level of its least component, that is assigned an SMR code for the level of maintenance under consideration (i.e., identified as maintenance significant).

Actions. Welding, grinding, riveting, straightening, facing, machining, and/or resurfacing.

11. Overhaul. That maintenance effort (service/action) prescribed to restore an item to a completely serviceable/operational condition as required by maintenance standards in appropriate technical publications. Overhaul is normally the highest degree of maintenance performed by the Army. Overhaul does not normally return an item to like new condition.
12. Rebuild. Consists of those services/actions necessary for the restoration of unserviceable equipment to a like new condition in accordance with original manufacturing standards. Rebuild is the highest degree of material maintenance applied to Army equipment. The rebuild operation includes the act of returning to zero those age measurements (hours/miles, etc.) considered in classifying Army equipment/components.

B-3. Explanation of Columns in the MAC, Section II.

Column (1) Group Number. Column (1) lists Functional Group Code (FCG) numbers, the purpose of which is to identify maintenance significant components, assemblies, subassemblies, and modules with the Next Higher Assembly (NHA).

Column (2), Component/Assembly. Column (2) contains the names of components, assemblies, subassemblies, and modules for which maintenance is authorized.

Column (3), Maintenance Function. Column (3) lists the functions to be performed on the item listed in column (2). (For detailed explanation of these functions refer to “Maintenance Functions” outlined above).

Column (4), Maintenance Level. Column (4) specifies each level of maintenance authorized to perform each function listed in column (3), by indicating work time required (expressed as manhours in whole hours or decimals) in the appropriate subcolumn. This work time figure represents the active time required to perform that maintenance function at the indicated level of maintenance. If the number or complexity of the tasks within the listed maintenance function varies at different maintenance levels, appropriate work time figures are to be shown for each level. The work time figure represents the average time required to restore an item (assembly, subassembly, component, module, end item, or system) to a serviceable condition under typical field operating conditions. This time includes preparation time (including any necessary disassembly/assembly time), troubleshooting/fault location time, and quality assurance time in addition to the time required to perform the specific tasks identified for the maintenance functions authorized in the MAC. The system designations for the various maintenance levels are as follows:

Field:

- C Operator or Crew maintenance
- O Unit maintenance
- F Direct Support maintenance

Sustainment:

- L Specialized Repair Activity
- H General Support maintenance
- D Depot maintenance

NOTE

The “L” maintenance level is not included in column (4) of the MAC. Functions to this level of maintenance are identified by work time figure in the “H” column of column (4), and an associated reference code is used in the REMARKS column (6). This code is keyed to the remarks and the SRA complete repair application is explained there.

Column (5), Tools and Equipment Reference Code. Column (5) specifies, by code, those common tool sets (not individual tools), common Test, Measurement and Diagnostic Equipment (TMDE), and special tools, special TMDE, and support equipment required to perform the designated function. Codes are keyed to the entries in the tools and test equipment table.

Column (6) Remarks Code. When applicable, this column contains a letter code, in alphabetic order, which is keyed to the remarks table entries.

B-4. Explanation of Columns in the Tools and Test Equipment Requirements, Section III.

Column (1) - Tool or Test Equipment Reference Code. The tool or test equipment reference code correlates with a code used in column (5) of the MAC.

Column (2) - Maintenance Level. The lowest level of maintenance authorized to use the tool or test equipment.

Column (3) - Nomenclature. Name or identification of tool or test equipment.

Column (4) - National Stock Number (NSN). The NSN of the tool or test equipment.

Column (5) - Tool Number. The manufacturer's part number.

B-5. Explanation of Columns in Remarks, Section IV.

Column (1) - Remarks Code. The code recorded in column (6) of the MAC.

Column (2) - Remarks. This column lists information pertinent to the maintenance function being performed as indicated in the MAC.

SECTION II. MAINTENANCE ALLOCATION CHART FOR SHELTER, ELECTRICAL EQUIPMENT S-280B/G AND S-280/G (SHIELDED)

(1) GROUP NUMBER	(2) COMPONENT/ ASSEMBLY	(3) MAINTENANCE FUNCTION	(4) MAINTENANCE LEVEL					(5) TOOLS AND EQUIPMENT REFERENCE CODE	(6) REMARKS
			FIELD		SUSTAINMENT				
			UNIT		DIRECT SUPPORT	GENERAL SUPPORT	DEPOT		
			C	O	F	H	D		
00	SHELTER, ELECTRICAL EQUIPMENT S-280B/G AND S-280B/G SHIELDED	Inspect Repair Repair	0.2		5.0				A
01	DOOR BRACE ASSEMBLY	Inspect Service Repair Replace	0.2	0.2 0.5 1.0				1 1	B
02	DOOR ASSEMBLY	Inspect Service Repair Repair Replace	0.2	0.2 0.5	4.0 2.0			1 1,2,3 1,2	B C D,E
0201	EMERGENCY EXIT PANEL ASSEMBLY	Inspect Service Repair Repair Replace	0.2	0.2 0.5 1.0	2.0			1 1,2,3 1	B C D,E

**SECTION II. MAINTENANCE ALLOCATION CHART
FOR
SHELTER, ELECTRICAL EQUIPMENT S-280B/G AND S-280/G (SHIELDED) - continued**

(1) GROUP NUMBER	(2) COMPONENT/ ASSEMBLY	(3) MAINTENANCE FUNCTION	(4) MAINTENANCE LEVEL					(5) TOOLS AND EQUIPMENT REFERENCE CODE	(6) REMARKS
			FIELD			SUSTAINMENT			
			UNIT		DIRECT SUPPORT	GENERAL SUPPORT	DEPOT		
			C	O	F	H	D		
0202	DOOR HANDLES, LOCKS/ LATCHES	Inspect Service Repair Replace	0.2	0.2 1.0 1.5				1 1	B
0203	AIR INLET FILTER	Inspect Replace	0.2	0.5				1,3	
03	TOWING BRACKET ASSEMBLIES	Inspect Service Repair Replace	0.2	0.5	0.5 4.0			1,2 1,2	B
04	LIFTING BRACKET ASSEMBLIES	Inspect Service Repair Replace	0.2	0.5	1.5 2.0			1,2 1,2	B
05	STEPS, HAND HOLDS, DRAIN PLUG	Inspect Service Replace	0.2	0.2 1.5					B
06	RFI/EMI COMPONENTS	Inspect Inspect Replace Replace	0.2	0.5	1.0 3.0			1,2 1,2	F E G
07	PANEL WALLS, FLOORS,CEILIN GS	Inspect Repair Repair Repair	0.2	0.5	2.5 8.0			1,2,3 1,2,3	C D H
08	SKID ASSEMBLY AND MOUNTING BRACKET	Inspect Replace	0.2		3.0			1,2	

**SECTION III. TOOL AND TEST EQUIPMENT REQUIREMENTS
FOR
SHELTER, ELECTRICAL EQUIPMENT S-280B/G AND S-280B/G (SHIELDED)**

(1) TOOL OR TEST EQUIPMENT REFERENCE CODE	(2) MAINTENANCE LEVEL	(3) NOMENCLATURE	(4) NATIONAL STOCK NUMBER	(5) TOOL NUMBER
1	O,F, H	Tool Kit, General Mechanics Automotive SC 5180-90-CL-N26	5180-00-177-7033	
2	F, H	Tool Kit, Electronic Equipment Shelter TK-144/G	5180-00-973-4369	
3	O,F, H	Riveter, Blind Hand	5120-00-017-2849	

SECTION IV. REMARKS

(1) REMARKS CODE	(2) REMARKS
A	Replace drip molding, plates, hinges, door stop angle, floor tread
B	Lubricate, touchup paint
C	Temporary repair of skin damage
D	Permanent repair of minor skin damage
E	Replace intake louver, RFI filter, drip cap, knobs, weather gaskets, hinges
F	Replace RFI/EMI washer
G	Replace RFI/EMI gasket
H	Repair of major skin damage with foam core damage

APPENDIX C

COMPONENTS OF END ITEM AND BASIC ISSUE ITEMS LISTS

Section I INTRODUCTION

C-1. Scope.

This appendix lists components of end item and basic issue items for the S-280B/G and S-280B/G Shielded shelters to help you inventory items required for safe and efficient operation.

C-2. General.

The Components of End Item and Basic Issue Items Lists are divided into the following sections:

a. Section II. Components of End. This listing is for information purposes only, and is not authority to requisition replacements. These items are part of the end item, but are removed and separately packaged for transportation or shipment. As part of the end item, these items must be with the end item whenever it is issued or transferred between property accounts. Illustrations are furnished to assist you in identifying the items.

b. Section III. Basic Issue Item. These are the minimum essential items required to place the shelter in operation, to operate it, and to perform emergency repairs. Although shipped separately packaged, BII must be with the shelter during operation and whenever it is transferred between property accounts. The illustrations will assist you with hard-to-identify items. This manual is your authority to request/requisition replacement BII, based on TOE/MTOE authorization of the end item.

C-3. Explanation of Columns.

The following provides an explanation of columns found in the tabular listings:

a. Column (1) - Illustration Number (Illus Number). This column indicates the number of the illustration in which the item is shown.

b. Column (2) - National Stock Number. Indicates the National stock number assigned to the item and will be used for requisitioning purposes.


c. Column (3) - Description. Indicates the Federal item name and, if required, a minimum description to identify and locate the item. The last line for each item indicates the FSCM (in parentheses) followed by the part number. If item needed differs for different models of this equipment, the model is shown under the "Usable On" heading in this column. These codes are identified as follows:

Code	Used On
A	Model S-280B/G
B	Model S-280B/G Shielded

d. Column (4) - Unit of Measure (U/M). Indicates the measure used in performing the actual operational/maintenance function. This measure is expressed by a two-character alphabetical abbreviation (e.g., ea, in, pr).

e. Column (5) - Quantity required (Qty rqr). Indicates the quantity of the item authorized to be used with/on the equipment.


Section II. COMPONENTS OF END ITEM

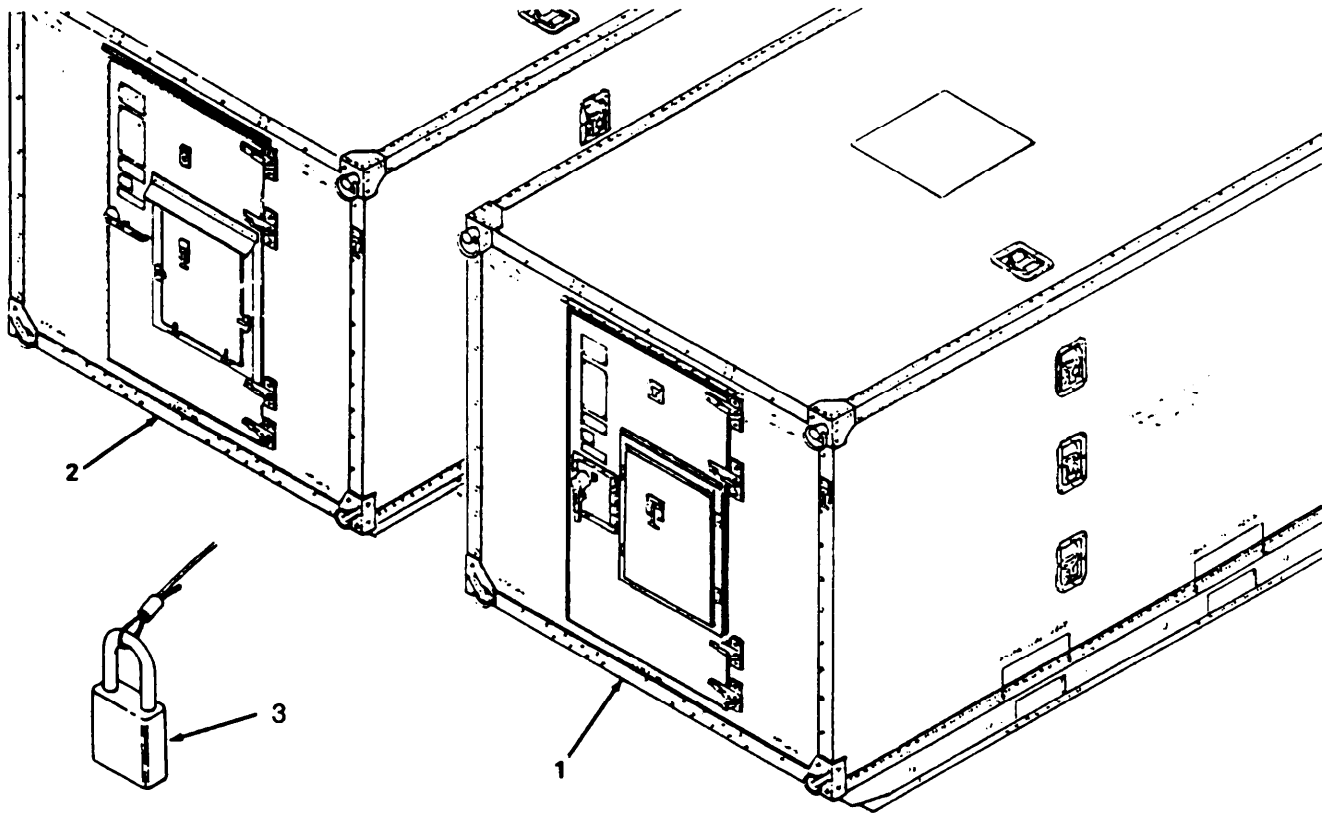

4753-043

(1) Illus Number	(2) National Stock Number	(3) Description FSCM and Part Number	Usable On Code	(4) U/M	(5) Qty Rqr
1	5410-00-117-2868	SHELTER, ELECTRICAL EQUIPMENT S-280B/G (80063) SM-D-200131	A	EA	1
2	5410 -00-001-4093	SHELTER, ELECTRICAL EQUIPMENT S-280B/G (SHIELDED) (80063) SM-D-200131	B	EA	1
3	5340-01-239-8705	PADLOCK AND KEY (80063) SC-C-595537	A,B	EA	1

Section III. BASIC ISSUE ITEMS

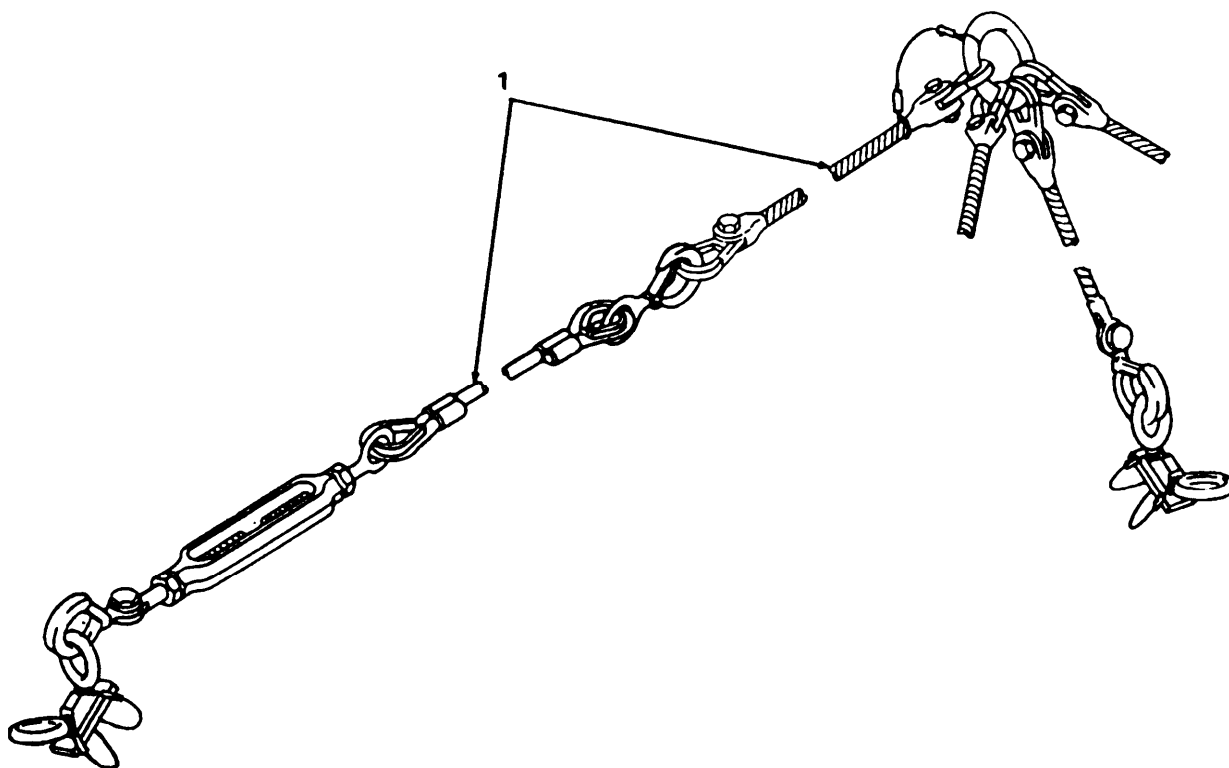

4753-044

(1) Illus Number	(2) National Stock Number	(3) Description FSCM and Part Number	Usable On Code	(4) U/M	(5) Qty Rqr
1		HOLD DOWN ASSEMBLY (80063) SC-D-36423		EA	1

APPENDIX D

EXPENDABLE/DURABLE SUPPLIES AND MATERIALS LIST

Section I. INTRODUCTION

D-1. Scope.

This appendix lists expendable supplies and materials you will need to operate and maintain the shelters. This listing is for information purposes only and is not authority to requisition the listed items. These items are authorized to you by CTA 50-970, Expendable Items (Except Medical, Class V, Repair Parts, and Heraldic Items), or CTA 8-100, Army Medical Department Expendable/Durable Items.

D-2. Explanation of Columns.

- a. Column (1) – Item Number. This number is assigned to the entry in the listing.
- b. Column (2) – Level. This column identifies the lowest level of maintenance that requires the listed item.

(enter as applicable)

- C - Operator
- O - Unit Maintenance
- F - Direct Support Maintenance
- H - General Support Maintenance

c. Column (3) - National Stock Number. This the National stock number assigned to the item; use it to request or requisition the item.

d. Column (4) - Description. Indicates the Federal item name, and, if required, a description to identify the item. The last line for each item indicates the Federal Supply Code for Manufacturer (FSCM) in parentheses followed by the part number.

e. Column (5) - Unit of Measure (U/M). Indicates the measure used in performing the actual maintenance function. This measure is expressed by a two-character alphabetical abbreviation (e.g., ea, in, pr). If the unit of measure differs from the unit of issue, requisition the lowest unit of issue that will satisfy your requirements.

Section II. EXPENDABLE/DURABLE SUPPLIES AND MATERIALS

(1) Item Number	(2) Level	(3) National stock number	(4) Description	(5) U/M
1	F	8040-00-016-8662	Adhesive, epoxy, hysol	bx
2	O	8040-00-952-3520	Adhesive, silicone rubber, 6 oz. tube	oz
3	O	8040-00-851-0211	Adhesive, silicone rubber, 5 oz. tube (black)	oz
4	O	8040-00-865-8991	Adhesive, silicone rubber, 12 oz. can (black)	oz

EXPENDABLE/DURABLE SUPPLIES AND MATERIALS (cont)

(1) Item Number	(2) Level	(3) National stock number	(4) Description	(5) U/M
5	O	8040-00-142-9823	Adhesive, silicone rubber, 12 oz. can (aluminum)	oz
6	F	8040-01-035-7848	Adhesive kit, two part, metal to metal	
7	F		Aluminum sheet, .040 in. thick QQ-A-250/11 6061-T6	
8	F		Aluminum sheet, .040 in. thick QQ-A-200/8 5052-H34	
9	O	8305-00-267-3015	Cloth, cheesecloth	yd
10	O	8305-00-205-3496	Cloth, cheesecloth, CCC-440, Type II, Class 2	yd
11	O		Conductive compound (80063) SM-D-555530-25 or SC-D-200140-12	
12	O	8415-00-634-4658	Gloves, leather	pr
13	F		Gasket (80063) SM-D-450461-4, SM-D-450462-7 or -8, and SM-B-555582	
14	F		Grease, Iubriplate (130-AA) (80063) SM-D-649953-5	
15	H		Insulation, closed cell rigid urethane foam, MIL-C-83400 or polystyrene foam, MIL-S-55286	
16	O	9150-00-823-7860	Lubricant, MIL-C-83300	
17	O	9550-00-402-4478	Lubricant, MIL-L-23398	
18	O		Lubricant, silicone, MIL-S-8660	
19	F	7220-00-254-4240	Matting, rubber floor, 1/8 in. thick	
20	F	7220-00-965-4699	Matting, tubber floor, 3/16 in. thick	
21	O		Paint, lusterless green enamel, MIL-E-46061 (S-280A/G) or Paint, lusterless green, no 383, polyurethane, MIL-C-46168 (S-280B/G)	gl
22	O		Paint, polyamide epoxy, MIL-C-22750	gl

EXPENDABLE/DURABLE SUPPLIES AND MATERIALS (cont)

(1) Item Number	(2) Level	(3) National stock number	(4) Description	(5) U/M
23	F	8030-00-845-4304	Primer for silastic TRV891, 1 pint can black	pt
24	F	9320-00-202-4008	Rubber, solid sheet, 1/8 in. thick	
25	F	9320-00-621-5409	Rubber, solid sheet, 1/8 in. thick	
26	O	5350-00-192-9318	Sandpaper, grit no. 40	
27	O	5350-00-192-5046	Sandpaper, grit no. 60	
28	O	5350-00-192-5047	Sandpaper, grit no. 80	
29	O	8030-00-753-5005	Sealing compound, 6 oz, MIL-S-8802	oz
30	O	8030-00-081-2333	Sealing compound, MIL-S-22473	
31	H	8030-00-275-8110	Sealing compound, 2-part kit, resin with catalyst	
32	O	5970-00-543-1005	Tape, electrically conductive	
33	O	7510-00-266-6712	Tape, masking, 1 in. wide	
34	O	7510-00-266-6714	Tape, masking, 1 1/2 in. wide	
35	O	7510-00-266-6712	Tape, pressure-sensitive adhesive, 2 in. wide	
36	F	8010-00-160-5794	Thinner, synthetic resin enamel, IT-T-306	
37	O	6610-00-579-8431	Toluene, technical grade solvent, TT-T-548	
38	O	4240-00-052-3776	Goggles, Industrial	pr

INDEX

Subject	Paragraph
A	
Abbreviations	1-6
Adjustments, initial	2-4
Administrative Storage	3-24
Air Inlet Filters	
Replacement	3-16
Service	3-16
Assembly and Preparation for Use	2-3
B	
Basic Issue Items	C-1
Blind Rivets, Installation and Removal	3-9
C	
Ceiling Panel, Repair	4-20, 5-10
Characteristics, Capabilities and Features	1-7
Component Location and Description	1-8
Components of End Item	C-1
D	
D-Ring Assemblies	
Replacement	3-18
Service	3-18
Data, Equipment	1-10
Data Plates, Replacement	4-8
Destruction of Army Material to Prevent Enemy Use	1-4
Differences Between Models	1-9
Direct Support Maintenance Procedures	4-5
Door Assembly	
Repair, Direct Support	4-11
Replacement, General Support	5-6
Service and Repair, Unit	3-12
Door Brace Assembly	
Repair	3-11
Replacement	3-11
Service	3-11
Door Knob Assembly, Replacement	4-16
Door Latch Assembly	
Repair	3-15
Replacement	3-15
Door Skin, Repair	4-18
Door Stop Angle, Replacement	4-9
Drain Plug, Replacement	3-19

D (cont)

Drip Cap, Replacement	4-13
Drip Mold, Replacement	4-7

E

Emergency Exit	
Latch Replacement	4-14
Repair	4-14
Strike Replacement	4-14
Stud Plate Assembly Relacement	4-14
Emergency Exit Panel Assembly	
Repair	3-13
Replacement	3-13
Service	3-13
Emergency Procedures	2-9
EMI Washer, Replacement	3-19
Expendable/Durable Supplies and Materials	D-1

F

Filter, RFI, Replacement	4-15
Filters, Air Inlet	
Replacement	3-16
Service	3-16
Floor Panel Repair	4-20
Floor Tread Replacement	4-10

G

Gaskets, Weather Replacement	4-12
General Support Maintenance Procedures	5-4

H

Hand Holds	
Replacement	3-18
Service	3-18

I

Initial Adjustment	2-4
Instruction Plates	2-7
Intake Louver Assembly, Replacement	4-15

J,K

INDEX (cont)

Subject	Paragraph
---------	-----------

L

Latch Assembly Door	
Repair	3-15
Replacement	3-15
Lifting Eye Assembly	
Repair	5-8
Replacement	5-8
Lifting Shelter	3-5
Loading Shelter Into ANSI/ISO Container	3-22
Loading Shelter Onto Truck	3-5
Lubrication Instructions	3-1

M

Maintenance Allocation Chart	B-4
Maintenance Forms and Records	1-2
Maintenance Procedures	
Direct Support	4-5
General Support	5-4
Unit	3-8
Marking, Shelter	1-11
Movement, Preparation For	2-6

N**O**

Operating Procedures	2-5
Operation in Unusual Weather	2-8

P

Painting, Touchup	3-10
Panel Assembly, Emergency Exit	
Repair	3-13
Replacement	3-13
Service	3-13
Panel Repair	
Permanent Patching	4-20, 5-10
Temporary (Tape).	3-9
Plates, Data, Replacement	4-8
Plates, instruction	2-7
Preparation for Movement	2-6
Preparation for Shipment and Storage	1-5
Preventive Maintenance Checks and Services, Operator	2-1

INDEX (cont)

Subject	Paragraph
Q	
R	
Recessed Step Pan Assembly	
Replacement	3-17
Service	3-17
References	A-1
Repair Parts	3-3, 4-3 , 5-3
Repair Procedures, General	3-9
Reporting Equipment Improvement Recommendations (EIR)	1-3
RFI Filter Replacement	4-15
RFI/EMI Components, Replacement	3-20, 4-19, 5-9
RFI/EMI Shielding Gasket Replacement	5-9
Rivet Installation and Removal	3-9
Rivnut Installation and Removal	3-9
S	
Safety, Care and Handling	1-12
Scope	1-1
Securing Shelter on Truck	3-5
Service Upon Receipt	3-5
Shielding Gasket, RFI/EMI Replacement	5-9
Shipment, Preparation For	1-5
Site Requirements	3-6
Skid Assembly, Replacement	5-11
Skid Mounting Bracket, Replacement	5-11
Skin, Door, Repair	4-18
Special Tools	3-2, 4-2, 5-2
Steps, Roof Access	
Replacement	3-17
Service	3-17
Storage, Administrative	3-24
Storage, Preparation For	1-5
Storage Requirements, General	3-23
Surface Preparation, Priming and Painting	4-6, 5-5
T	
T-Latches and Holders, Replacement	3-14
Towing Eye Assemblies	
Repair	5-7
Replacement	5-7
Tread, Floor, Replacement	4-10

INDEX (cont)

Subject	Paragraph
T (cont)	
Troubleshooting	
Direct Support	4-4
Unit	3-7
U	
Unit Maintenance Procedures	3-8
V	
W	
Washer, EMI, Replacement	3-19
X, Y, Z	

By Order of the Secretary of the Army:

Official:



MILTON H. HAMILTON

*Administrative Assistant to the
Secretary of the Army*

05411

GORDON R. SULLIVAN
*General, United States Army
Chief of Staff*

DISTRIBUTION:

To be distributed in accordance with DA Form 12-25-E, block no. 6169, requirements for
TM 10-5411-206-14.

These are the instructions for sending an electronic 2028

The following format must be used if submitting an electronic 2028. The subject line must be exactly the same and all fields must be included; however only the following fields are mandatory: 1, 3, 4, 5, 6, 7, 8, 9, 10, 13, 15, 16, 17, and 27.

From: "Whoever" <whoever@avma27.army.mil>

To: amssbriml@natick.army.mil

Subject: DA Form 2028

1. From: Joe Smith
2. Unit: home
3. Address: 4300 Park
4. City: Hometown
5. St: MO
6. Zip: 77777
7. Date Sent: 19-OCT-93
8. Pub no: 55-2840-229-23
9. Pub Title: TM
10. Publication Date: 04-JUL-85
11. Change Number: 7
12. Submitter Rank: MSG
13. Submitter FName: Joe
14. Submitter MName: T
15. Submitter LName: Smith
16. Submitter Phone: 123-123-1234
17. Problem: 1
18. Page: 2
19. Paragraph: 3
20. Line: 4
21. NSN: 5
22. Reference: 6
23. Figure: 7
24. Table: 8
25. Item: 9
26. Total: 123
27. Text:

This is the text for the problem below line 27.

RECOMMENDED CHANGES TO PUBLICATIONS AND BLANK FORMS For use of this form, see AR 25-30; the proponent agency is ODISC4.						Use Part II (reverse) for Repair Parts and Special Tool Lists (RPSTL) and Supply Catalogs/Supply Manuals (SC/SM).		DATE 21 October 2003	
TO: (Forward to proponent of publication or form) (Include ZIP Code) COMMANDER U.S. ARMY TANK-AUTOMOTIVE AND ARMAMENT COMMAND ATTN: AMSTA-LC-CECT 15 KANSAS STREET NATICK, MA 01760-5052						FROM: (Activity and location) (Include ZIP Code) <i>PFC Jane Doe</i> <i>CO A 3rd Engineer BR</i> <i>Ft. Leonardwood, MO 63108</i>			
PART I – ALL PUBLICATIONS (EXCEPT RPSTL AND SC/SM) AND BLANK FORMS									
PUBLICATION/FORM NUMBER TM 10-1670-296-23&P						DATE 30 October 2002		TITLE Unit Manual for Ancillary Equipment for Low Velocity Air Drop Systems	
ITEM NO.	PAGE NO.	PARA-GRAPH	LINE NO. *	FIGURE NO.	TABLE NO.	RECOMMENDED CHANGES AND REASON <i>(Provide exact wording of recommended changes, if possible).</i>			
	0036 00-2				1	<i>In table 1, Sewing Machine Code Symbols, the second sewing machine code symbol should be MD ZZ not MD 22.</i> <i>Change the manual to show Sewing Machine, Industrial: Zig-Zag; 308 stitch; medium-duty; NSN 3530-01-181-1421 as a MD ZZ code symbol.</i>			
<i>*Reference to line numbers within the paragraph or subparagraph.</i>									
TYPED NAME, GRADE OR TITLE Jane Doe, PFC					TELEPHONE EXCHANGE/AUTOVON, PLUS EXTENSION 508-233-4141			SIGNATURE Jane Doe <i>Jane Doe</i>	

TO: <i>(Forward direct to addressee listed in publication)</i> COMMANDER U.S. ARMY TANK-AUTOMOTIVE AND ARMAMENT COMMAND ATTN: AMSTA-LC-CECT 15 KANSAS STREET NATICK, MA 01760-5052					FROM: <i>(Activity and location) (Include ZIP Code)</i> <i>PFC Jane Doe</i> <i>CO A 3rd Engineer BR</i> <i>Ft. Leonardwood, MO 63108</i>			DATE 21 October 2003	
PART II – REPAIR PARTS AND SPECIAL TOOL LISTS AND SUPPLY CATALOGS/SUPPLY MANUALS									
PUBLICATION NUMBER TM 10-1670-296-23&P					DATE 30 October 2002		TITLE Unit Manual for Ancillary Equipment for Low Velocity Air Drop Systems		
PAGE NO.	COLM NO.	LINE NO.	NATIONAL STOCK NUMBER	REFERENCE NO.	FIGURE NO.	ITEM NO.	TOTAL NO. OF MAJOR ITEMS SUPPORTED	RECOMMENDED ACTION	
0066 00-1					4			<i>Callout 16 in figure 4 is pointed to a <u>D-Ring</u>. In the Repair Parts List key for figure 4, item 16 is called a <u>Snap Hook</u>. Please correct one or the other.</i>	
PART III – REMARKS <i>(Any general remarks or recommendations, or suggestions for improvement of publications and blank forms. Additional blank sheets may be used if more space is needed.)</i>									
TYPED NAME, GRADE OR TITLE				TELEPHONE EXCHANGE/AUTOVON, PLUS EXTENSION			SIGNATURE		

RECOMMENDED CHANGES TO PUBLICATIONS AND BLANK FORMS For use of this form, see AR 25-30; the proponent agency is ODISC4.						Use Part II (<i>reverse</i>) for Repair Parts and Special Tool Lists (RPSTL) and Supply Catalogs/Supply Manuals (SC/SM).	DATE
TO: (<i>Forward to proponent of publication or form</i>) (<i>Include ZIP Code</i>) COMMANDER U.S. ARMY TANK-AUTOMOTIVE AND ARMAMENT COMMAND ATTN: AMSTA-LC-CECT 15 KANSAS STREET NATICK, MA 01760-5052						FROM: (<i>Activity and location</i>) (<i>Include ZIP Code</i>)	
PART I - ALL PUBLICATIONS (EXCEPT RPSTL AND SC/SM) AND BLANK FORMS							
PUBLICATION/FORM NUMBER TM 10-5411-206-14				DATE 30 September 1993		TITLE Operator's, Unit, Direct Support and General Support Maintenance Manual for Shelter, Electrical Equipment	
ITEM NO.	PAGE NO.	PARA-GRAPH	LINE NO. *	FIGURE NO.	TABLE NO.	RECOMMENDED CHANGES AND REASON <i>(Provide exact wording of recommended changes, if possible).</i>	
<i>*Reference to line numbers within the paragraph or subparagraph.</i>							
TYPED NAME, GRADE OR TITLE				TELEPHONE EXCHANGE/AUTOVON, PLUS EXTENSION		SIGNATURE	

TO: <i>(Forward direct to addressee listed in publication)</i> COMMANDER U.S. ARMY TANK-AUTOMOTIVE AND ARMAMENT COMMAND ATTN: AMSTA-LC-CECT 15 KANSAS STREET NATICK, MA 01760-5052					FROM: <i>(Activity and location) (Include ZIP Code)</i>			DATE	
PART II – REPAIR PARTS AND SPECIAL TOOL LISTS AND SUPPLY CATALOGS/SUPPLY MANUALS									
PUBLICATION NUMBER TM 10-5411-206-14					DATE 30 September 1993			TITLE Operator's, Unit, Direct Support and General Support Maintenance Manual for Shelter, Electrical Equipment	
PAGE NO.	COLM NO.	LINE NO.	NATIONAL STOCK NUMBER	REFERENCE NO.	FIGURE NO.	ITEM NO.	TOTAL NO. OF MAJOR ITEMS SUPPORTED	RECOMMENDED ACTION	
PART III – REMARKS <i>(Any general remarks or recommendations, or suggestions for improvement of publications and blank forms. Additional blank sheets may be used if more space is needed.)</i>									
TYPED NAME, GRADE OR TITLE				TELEPHONE EXCHANGE/AUTOVON, PLUS EXTENSION			SIGNATURE		

RECOMMENDED CHANGES TO PUBLICATIONS AND BLANK FORMS For use of this form, see AR 25-30; the proponent agency is ODISC4.						Use Part II (reverse) for Repair Parts and Special Tool Lists (RPSTL) and Supply Catalogs/Supply Manuals (SC/SM).	DATE
TO: (Forward to proponent of publication or form) (Include ZIP Code) COMMANDER U.S. ARMY TANK-AUTOMOTIVE AND ARMAMENT COMMAND ATTN: AMSTA-LC-CECT 15 KANSAS STREET NATICK, MA 01760-5052						FROM: (Activity and location) (Include ZIP Code)	
PART I - ALL PUBLICATIONS (EXCEPT RPSTL AND SC/SM) AND BLANK FORMS							
PUBLICATION/FORM NUMBER TM 10-5411-206-14				DATE 30 September 1993		TITLE Operator's, Unit, Direct Support and General Support Maintenance Manual for Shelter, Electrical Equipment	
ITEM NO.	PAGE NO.	PARA-GRAPH	LINE NO. *	FIGURE NO.	TABLE NO.	RECOMMENDED CHANGES AND REASON (Provide exact wording of recommended changes, if possible).	
<i>*Reference to line numbers within the paragraph or subparagraph.</i>							
TYPED NAME, GRADE OR TITLE				TELEPHONE EXCHANGE/AUTOVON, PLUS EXTENSION		SIGNATURE	

TO: <i>(Forward direct to addressee listed in publication)</i> COMMANDER U.S. ARMY TANK-AUTOMOTIVE AND ARMAMENT COMMAND ATTN: AMSTA-LC-CECT 15 KANSAS STREET NATICK, MA 01760-5052					FROM: <i>(Activity and location) (Include ZIP Code)</i>			DATE	
PART II – REPAIR PARTS AND SPECIAL TOOL LISTS AND SUPPLY CATALOGS/SUPPLY MANUALS									
PUBLICATION NUMBER TM 10-5411-206-14					DATE 30 September 1993			TITLE Operator's, Unit, Direct Support and General Support Maintenance Manual for Shelter, Electrical Equipment	
PAGE NO.	COLM NO.	LINE NO.	NATIONAL STOCK NUMBER	REFERENCE NO.	FIGURE NO.	ITEM NO.	TOTAL NO. OF MAJOR ITEMS SUPPORTED	RECOMMENDED ACTION	
PART III – REMARKS <i>(Any general remarks or recommendations, or suggestions for improvement of publications and blank forms. Additional blank sheets may be used if more space is needed.)</i>									
TYPED NAME, GRADE OR TITLE				TELEPHONE EXCHANGE/AUTOVON, PLUS EXTENSION			SIGNATURE		

The Metric System and Equivalents

Linear Measure

1 centimeter = 10 millimeters = .39 inch
 1 decimeter = 10 centimeters = 3.94 inches
 1 meter = 10 decimeters = 39.37 inches
 1 dekameter = 10 meters = 32.8 feet
 1 hectometer = 10 dekameters = 328.08 feet
 1 kilometer = 10 hectometers = 3,280.8 feet

Weights

1 centigram = 10 milligrams = .15 grain
 1 decigram = 10 centigrams = 1.54 grains
 1 gram = 10 decigrams = .035 ounce
 1 dekagram = 10 grams = .35 ounce
 1 hectogram = 10 dekagrams = 3.52 ounces
 1 kilogram = 10 hectograms = 2.2 pounds
 1 quintal = 100 kilograms = 220.46 pounds
 1 metric ton = 10 quintals = 1.1 short tons

Liquid Measure

1 centiliter = 10 milliliters = .34 fl. ounce
 1 deciliter = 10 centiliters = 3.38 fl. ounces
 1 liter = 10 deciliters = 33.81 fl. ounces
 1 dekaliter = 10 liters = 2.64 gallons
 1 hectoliter = 10 dekaliters = 26.42 gallons
 1 kiloliter = 10 hectoliters = 264.18 gallons

Square Measure

1 sq. centimeter = 100 sq. millimeters = .15 sq. inch
 1 sq. decimeter = 100 sq. centimeters = 15.5 sq. inches
 1 sq. meter (centare) = 100 sq. decimeters = 10.76 sq. feet
 1 sq. dekameter (are) = 100 sq. meters = 1,076.4 sq. feet
 1 sq. hectometer (hectare) = 100 sq. dekameters = 2.47 acres
 1 sq. kilometer = 100 sq. hectometers = .386 sq. mile

Cubic Measure

1 cu. centimeter = 1000 cu. millimeters = .06 cu. inch
 1 cu. decimeter = 1000 cu. centimeters = 61.02 cu. inches
 1 cu. meter = 1000 cu. decimeters = 35.31 feet

Approximate Conversion Factors

<i>To change</i>	<i>To</i>	<i>Multiply by</i>	<i>To change</i>	<i>To</i>	<i>Multiply by</i>
inches	centimeters	2.540	ounce-inches	newton-meters	.007062
feet	meters	.305	centimeters	inches	.394
yards	meters	.914	meters	feet	3.280
miles	kilometers	1.609	meters	yards	1.094
square inches	square centimeters	6.451	kilometers	miles	.621
square feet	square meters	.093	square centimeters	square inches	.155
square yards	square meters	.836	square meters	square feet	10.764
square miles	square kilometers	2.590	square meters	square yards	1.196
acres	square hectometers	.405	square kilometers	square miles	.386
cubic feet	cubic meters	.028	square hectometers	acres	2.471
cubic yards	cubic meters	.765	cubic meters	cubic feet	35.315
fluid ounces	milliliters	29.573	cubic meters	cubic yards	1.308
pints	liters	.473	milliliters	fluid ounces	.034
quarts	liters	.946	liters	pints	2.113
gallons	liters	3.785	liters	quarts	1.057
ounces	grams	28.349	liters	gallons	.264
pounds	kilograms	.454	grams	ounces	.035
short tons	metric tons	.907	kilograms	pounds	2.205
pound-feet	newton-meters	1.356	metric tons	short tons	1.102
pound-inches	newton-meters	.11296			

Temperature (Exact)

_F	Fahrenheit	5/9 (after	Celsius	_C
	temperature	subtracting 32)	temperature	

PIN: 071888-000

This fine document...

Was brought to you by me:



[Liberated Manuals -- free army and government manuals](#)

Why do I do it? I am tired of sleazy CD-ROM sellers, who take publicly available information, slap “watermarks” and other junk on it, and sell it. Those masters of search engine manipulation make sure that their sites that sell free information, come up first in search engines. They did not create it... They did not even scan it... Why should they get your money? Why are not letting you give those free manuals to your friends?

I am setting this document FREE. This document was made by the US Government and is NOT protected by Copyright. Feel free to share, republish, sell and so on.

I am not asking you for donations, fees or handouts. If you can, please provide a link to liberatedmanuals.com, so that free manuals come up first in search engines:

<A HREF=<http://www.liberatedmanuals.com/>>Free Military and Government Manuals

- Sincerely
Igor Chudov
<http://igor.chudov.com/>
- [Chicago Machinery Movers](#)